

REFERENCES

- AD633 Data Sheet, *Analog Devices, Inc.*, 1999.
- Alexeev V.L., Das S., Finegold D.N., and Asher S.A., Photonic crystal glucose-sensing material for noninvasive monitoring of glucose in tear fluid, *Clin. Chem.*, 50, 2353–2360, 2004.
- Altman DG (1991) Practical statistics for medical research. *London: Chapman and Hall.*
- American Diabetes Association (2014), Diagnosis and classification of Diabetes mellitus. *Diabetes Care*, 37, S81-S90, 2014.
- American Diabetes Association (2014), Standards of medical care in diabetes, *Diabetes Care*, 37(1), S14-S80, 2014.
- American Heart Association (2011), *Understanding blood pressure readings*, 11, January, 2011.
- Amir Orna, Daphna Weinstein, Silviu Zilberman, Malka Less, Daniele Perl-Treves, Harel Primack, Aharon Weinstein, Efi Gabis, Boris Fikhte, Avraham Karasik, Continuous Noninvasive Glucose Monitoring Technology Based on Occlusion Spectroscopy, *J Diabetes Sci. Technol.*, 1(4), 463-469. 2007.
- Animas Glucowatch, *Diabetes Services, Inc.*, 2005.
- Ansari, RR, Bockle, S and Rovati, L, New optical scheme for a polarimetric-based glucose sensor, *Journal of Biomedical Optics*, 9, 103-115, 2004.
- Armitage P, Berry G, Matthews JNS., Statistical methods in medical research. 4th ed. *Blackwell Science.*, 2002.
- Arnold, SA, Harvey, LM, McNeil, B and Hall, JW, Employing Near-Infrared Spectroscopic Methods of Analysis for Fermentation Monitoring and Control, Part 1, Method Development, *BioPharm International*, 2002.
- Arnold M.A., Non-invasive glucose monitoring, *Curr. Opin. Biotechnol.*, 7, 46–49, 1996.
- Assendelft O.W., Spectrophotometry of Hemoglobin Derivates, *Royal Vangorcum Ltd., Assen*, 1970.
- Ballerstadt, R and Schultz, JS, A Fluorescence Affinity Hollow Fiber Sensor for Continuous Transdermal Glucose Monitoring, *Anal. Chem.*, 72, 4185-4192, 2000.
- Bashkatov A.N., Zhestkov D.M., Genina E.A., Immersion clearing of human blood in the visible and near-infrared spectral regions, *Opt. Spectr.*, vol. 98, 2005, 638-646, 2005.
- Bartle, Sherbert, Introduction to real analysis (4th ed.), *John Wiley & Sons*, ISBN 978-0-471-43331-6, 2011.
- Bates, H.M., *Laboratory Management*, 16, 1978.
- Beckers Ingeborg, Spectral response of glucose: spectral response within optical window of tissue, *ANDOR an Oxford Instruments company*, 2013.

- Benyon, S, Metabolism and Nutrition, *Elsevier Science Ltd, London*, 1-2, 2003.
- Berger, AJ, Itzkan, I and Feld, MS, Feasibility of measuring blood glucose concentration by near-infrared Raman spectroscopy, *Spectrochimica Acta Part A*, 53, 287-292, 1997.
- Birnbaum Y, Luo H, Nagai T, Fishbein MC, Peterson TM, Li S, Noninvasive In Vivo Clot Dissolution Without a Thrombolytic Drug Recanalization of Thrombosed Iliofemoral Arteries by Transcutaneous Ultrasound Combined With Intravenous Infusion of Microbubbles, *Circulation*, 97,130-134, 1998.
- Bill Jelen, Excel 2013 In Depth, *Que Publishing*, 2013.
- Bina, DM, Anderson, RL, Johnson, ML, Bergenstal, RM and Kendall, DM, Clinical Impact of Prandial State, Exercise, and Site Preparation on the Equivalence of Alternative-Site Blood Glucose Testing, *Diabetes Care*, 26, 981-985, 2003.
- Bin Zainul Abidin M.T, Rosli M.K.R., Shamsuddin S.A., Madzhi N.K, Abdullah Md., Initial Quantitative Comparison of 940 nm and 950 nm Infrared Sensor Performance for Measuring Glucose Non-invasively, *Proc. of the IEEE International Conference on Smart Instrumentation, Measurement and Applications (ICSIMA)*, Kuala Lumpur, Malaysia, 25-27, November, 2013.
- Bland M., An introduction to medical statistics, 3rd ed. *Oxford: Oxford University Press.*, 2000.
- Bland JM, Altman DG., Measuring agreement in method comparison studies. *Statistical Methods in Medical Research*, 8, 135-160, 1999.
- Bland JM, Altman DG., Statistical method for assessing agreement between two methods of clinical measurement, *The Lancet*, 307-310, 1986.
- Blank TB, Ruchti TL, Lorenz AD, Monfre SL, Makarewicz MR, Mattu M, Hazen KH: Clinical results from non-invasive blood glucose monitor. *Proc SPIE*, 4624, 1–10, 2002.
- Bockle S., Rovati L., Ansari R.R., Polarimetric glucose sensing using the Brewster-reflection off-eye lens: theoretical analysis, *Proc. SPIE*, 4624,160–164, 2002.
- Boehm Harman-I, Gal A, Raykhman AM, Zahn JD, Naidis E, Mayzel Y, Noninvasive glucose monitoring: a novel approach, *J Diabetes Sci Technol.*, 3(2), 253–260, 2009.
- Boehm Harman-I, Gal A, Raykhman AM, Naidis E, Mayzel Y, Noninvasive Glucose Monitoring: Increasing Accuracy by Combination of Multi-Technology and Multi-Sensors, *J Diabetes Sci Technol.*, 4(3), 583-595, 2010.
- Boer Ian H. de, Bryan Kestenbaum, Tessa C. Rue, Michael W. Steffes, Patricia A. Cleary MS, Mark E. Molitch, et al. , Insulin Therapy, Hyperglycemia, and Hypertension in Type 1 Diabetes Mellitus, for the Diabetes Control and Complications Trial (DCCT)/Epidemiology of Diabetes Interventions and Complications (EDIC) Study Research Group, *Arch Intern Med.*, 168(17),1867-1873, 2008.
- Bookchin RM, Gallop PM, Structure of haemoglobin A1c: nature of the N-terminal beta chain blocking group, *Biochem. Biophys. Res. Commun.* 32 (1), 86–93, 1968.

- Bunn HF, Haney DN, Gabbay KH, Gallop PM., Further identification of the nature and linkage of the carbohydrate in haemoglobin A1c. *Biochem. Biophys.Res. Commun.*, 67 (1), 103–109, 1975.
- Burmeister, JJ, Arnold, MA and Small, GW, Noninvasive blood glucose measurements by near-infrared transmission spectroscopy across human tongues, *Diabetes Technol Ther*, 2, 5-16, 2000.
- Burmeister, JJ and Arnold, MA, Evaluation of Measurement Sites for Noninvasive Blood Glucose Sensing with Near-Infrared Transmission Spectroscopy, *Clin Chem*, 45, 1621-1627, 1999.
- Burmeister, JJ and Arnold, MA, Spectroscopic Considerations for Noninvasive Blood Glucose Measurements with Near Infrared Spectroscopy, *IEEE*, 1998.
- B5B-940-8, Infrared LED 940 nm, *Data sheet of Roithner LaserTechnik*, Vienna, Austria.
- Caduff A, Mueller M, Megej A, Dewarrat F, Suri R. E., Klisic J, Donath M, Zakharov P, Schaub D, Stahel W. A., Talary Mark S., Characteristics of a multisensor system for non invasive glucose monitoring with external validation and prospective evaluation, *Biosensors and Bioelectronics*, 26, 3794–3800, 2011.
- Caduff A, Dewarrat F, Talary M, et al., Non-invasive glucose monitoring in patients with diabetes: a novel system based on impedance spectroscopy, *Biosens Bioelectron.*, 22, 598-604, 2006.
- Caduff A, Hirt E, Feldman Y, Ali Z, Heinemann L. First human experiments with a novel non-invasive, non-optical continuous glucose monitoring system. *Biosens Bioelectron.*, 19(3), 209–217, 2003.
- Caduff A, Talary MS, Mueller M, et al. Non-invasive glucose monitoring in patients with Type 1 diabetes: a multisensor system combining sensors for dielectric and optical characterisation of skin. *Biosens Bioelectron.*, 24(9), 2778–2784, 2009.
- Chandalia H. B., Krishnaswamy P. R, Glycated Haemoglobin. *Current Science*, 83 (12), 1522-1532, 2002.
- Chen CS, Wang KK, Jan MY, et al., Noninvasive blood glucose monitoring using the optical signal of pulsatile microcirculation: a pilot study in subjects with diabetes. *J Diabetes Complications*, 22, 371-376, 2008.
- Chen, W, Liu, R, Xu, K and Wang, RK, Influence of contact state on NIR diffuse reflectance spectroscopy in vivo, *Journal of Physics D: Applied Physics*, 38, 2691-2695, 2005.
- Choleau, C, Dokladal, P, Klein, J-C, Ward, WK, Wilson, GS and Reach, G, Prevention of Hypoglycemia Using Risk Assessment With a Continuous Glucose Monitoring System, *Diabetes*, 51, 3263-3273, 2002.
- Cho O.K., Kim Y.O., Mitsumaki H., Kuwa K., Noninvasive measurement of glucose by metabolic heat conformation method, *Clin Chem*, 50, 1894–1898, 2004.

- Chowdhury, M.K., Srivastava, A., Sharma, N., Sharma, S., 'Noninvasive blood glucose measurement utilizing a newly designed system based on modulated ultrasound and infrared light', *International Journal of Diabetes in Developing Countries; Springer*, 1-10, December 2015.
- Chowdhury, M.K., Srivastava, A., Sharma, N., Sharma, S., Neeraj Sharma, Prospective Analysis of Developing Noninvasive Blood Glucose Monitoring Biosensors for Diabetic Population, *Bioscience Biotechnology Research Asia*, Vol. 11(3), 1639-1647, 2014.
- Chowdhury, M.K., Srivastava, A., Sharma, N., Sharma, S., 'Challenges & Countermeasures in Optical Noninvasive Blood Glucose Detection', *International Journal of Innovative Research in Science, Engineering and Technology (IJIRSET)*, Vol.2, Issue 1, 324-329, Jan 2013.
- Clarke W. L., Gonder-Frederick L. Carter A., W., Pohl S. L., Evaluating clinical accuracy of systems for self-monitoring of blood glucose, *Diabetes Care*, 10(5), 622-628, 1987.
- Clarke W. L., Kovatchev B., Continuous Glucose Sensors: Continuing Questions about Clinical Accuracy, *Journal of Diabetes Science and Technology*, 1 (5), 669-675, 2007.
- Coakley W.T, Ultrasonic separations in analytical biotechnology, *Trends in Biotechnology*, 15, 506-511, 1997.
- Cornbleet PJ, Gochman N., Incorrect least-squares regression coefficients in method-comparison analysis. *Clinical Chemistry*, 25, 432-438, 1979.
- Collins PM., Carbohydrates. *Chapman and Hall, London*, 1987.
- Cote, D and Vitkin, IA, Balanced detection for low-noise precision polarimetric measurements of optically active, multiply scattering tissue phantoms, *Journal of Biomedical Optics*, 9, 213-220, 2004.
- Cote G.L., Fox M.D., Northrop R.B., Noninvasive optical polarimetric glucose sensing using a true phase technique, *IEEE Trans. Biomed. Eng.*, 39(7), 752-756, 1992.
- Danaei G., Finucane M. M., Lu Y., Singh G. M., Cowan M. J., Paciorek C. J., Lin J. K., Farzadfar F., Khang Y. H., Stevens G. A., Rao M., Ali M. K., Riley L. M., Robinson C. A., and Ezzati M., National, regional, and global trends in fasting plasma glucose and diabetes prevalence since 1980: systematic analysis of health examination surveys and epidemiological studies with 370 country-years and 2·7 million participants, *Lancet*, 31, 378, 2011.
- Duck FA., Physical Properties of Tissue: a Comprehensive Reference Book. *Academic Press Inc.*, San Diego, 1990.
- Duncan, A, Hannigan, J, Freeborn, SS, Rae, PW, McIver, B, Greig, F, Johnston, EM, Binnie, DT and MacKenzie, HA, A Portable Non-invasive Blood Glucose Monitor, *The 8th International Conference On Solid-State Sensors And Actuators And Eurosensors IX*, 1995.
- The Diabetes Control and Complications Trial Research Group (DCCT), The effect of intensive treatment of diabetes on the development and progression of long-term complications in insulin-dependent diabetes mellitus, *N Engl J Med.*, 329 (14), 977-86, 1993.

- Ediger MN, Olson BP, Maynard JD., Noninvasive optical screening for diabetes. *J Diabetes Sci Technol.*, **3**, 776–780, 2009.
- Enejder A.M.K., Seccina T.G., Oh J., Hunter M., Shih W.C., Sasic S., Horowitz G.L., Feld M.S., Raman spectroscopy for noninvasive glucose measurements, *J. Biomed. Opt.*, **10**, 031114, 2005.
- Esenaliev R.O., Larin K.V., Larina I.V., et al., Noninvasive monitoring of glucose concentration with optical coherence tomography, *Opt. Lett.*, **26**, 992–994, 2001.
- EPD-1300-5.3, Infrared Detector, *Data sheet of Roithner LaserTechnik*, Vienna, Austria.
- Facchinetti A, Sparacino G, and Cobelli C, Reconstruction of Glucose in Plasma from Interstitial Fluid Continuous Glucose Monitoring Data: Role of Sensor Calibration, *J Diabetes Sci Technol.*, **1**(7), 617-627, 2007.
- Fatemi M., Greenleaf J. F., Vibro-acoustography: An imaging modality based on ultrasound stimulated acoustic emission, *Proc. Natl. Acad. Sci. U.S.A.*, **96**, 6603–6608, 1999.
- Filipovský J, Ducimetière P, Eschwège E, Richard JL, Rosselin G, Claude JR., The relationship of blood pressure with glucose, insulin, heart rate, free fatty acids and plasma cortisol levels according to degree of obesity in middle-aged men, *J Hypertens.*, Feb, **14**(2), 229-235, 1996.
- Fujimoto, JG, Optical Coherence Tomography: Introduction, Handbook of Optical Coherence Tomography, Eds.: b. E. Bouma and G. J. Tearney), *Marcel Dekker, Inc*, New York, 1-3, 2002.
- Flock ST, Jacques SL, Wilson BC., Star WM, Van Gemert MJC, Optical Properties of Intralipid: A phantom medium for light propagation studies, *Lasers in Surgery and Medicine*, **12**, 510-519, 1992.
- Frenzel L.E Jr. (Editor), Principles of Electronics Communications Systems, Third Edition, *The McGraw-Hill Companies*, Chapter 3, 93-117, 2008.
- Gabbay RA, Sivarajah S., Optical coherence tomography based continuous noninvasive glucose monitoring in patients with diabetes, *Diabetes Technol Ther.*, **10**, 188-193, 2008.
- Gandrud, LM, Paguntalan, HU, Van Wyhe, MM, Kunselman, BL, Leptien, AD, Wilson, DM, Eastman, RC and Buckingham, BA, Use of the Cygnus GlucoWatch biographer at a diabetes camp, *Pediatrics*, **113**, 108-111, 2004.
- Gebhart, S, Faupel, M, Fowler, R, Kapsner, C, Lincoln, D, McGee, V, Pasqua, J, Steed, L, Wangsness, M, Xu, F and Vanstony, M, Glucose sensing in transdermal body fluid collected under continuous vacuum pressure via micropores in the stratum corneum, *Diabetes Technol Ther*, **5**, 159-166, 2003.
- Goldsmith LA., Physiology, Biochemistry and Molecular Biology of the Skin. 2nd edition, *Oxford University Press*, 1991.
- Gourzi M, Rouane A, Guelaz R, et al. Non-invasive glycaemia blood measurements by electromagnetic sensor: study in static and dynamic blood circulation. *J Med Eng Technol.*, **29**(1), 22–26, 2005.

- Greenslade T.B., Experiments with ultrasonic transducers, *Physical Teacher*, 32 (October), 392-397, 1994.
- Guevara E., Gonzalez F. J., Joint optical-electrical technique for noninvasive glucose monitoring, *Revista Mexicana De Fisica*, 56(5), 430-434, 2010.
- Guevara E., Gonzalez F. J., Prediction of Glucose Concentration by Impedance Phase Measurements, in *MEDICAL PHYSICS: Tenth Mexican Symposium on Medical Physics, Mexico City (Mexico)*, 1032, 259-261, 2008.
- Hathout, E. Patel, N, Southern, C, Hill, J, Anderson, R, Sharkey, J, Hadley-Scofield, M, Tran, L, Leptien, A, Lopatin, M, Wang, B, Mace, J and Eastman, R, Home use of the GlucoWatch G2 biographer in children with diabetes, *Pediatrics*, 115, 662-666, 2005.
- Holman Rury R., Paul S. K., Bethel M. A, H. A. W. Neil, and David R. M, Long-Term Follow-up after Tight Control of Blood Pressure in Type 2 Diabetes, *N Engl. J Med.*, 359, 1565-1576, 2008.
- Hariri Ali, Wang Le Yi., Identification and low-complexity regime-switching-insulin control of type I diabetic patients, *J. Biomedical Science and Engineering*, 4, 297-314, 2011.
- Heise, HM, Bittner, A and Marbach, R, Clinical chemistry and near infrared spectroscopy: technology for non-invasive glucose monitoring, *Journal of Near Infrared Spectroscopy*, 6, 349-359, 1998.
- Heise, HM, Bittner, A and Marbach, R, Near-infrared reflectance spectroscopy for noninvasive monitoring of metabolites, *Clin Chem Lab Med*, 38,137-145, 2000.
- Heise, HM and Lampen, P, Transcutaneous glucose measurements using near-infrared spectroscopy: validation of statistical calibration models, *Diabetes Care*, 23, 1208-1210, 2000.
- Heise, HM, Marbach, R, Janatsch, G and Kruse-Jarres, JD, Multivariate determination of glucose in whole blood by attenuated total reflection infrared spectroscopy, *Anal Chem*, 61, 2009-2015, 1989.
- Heise, HM and Marbach, R, Human oral mucosa studies with varying blood glucose concentration by non-invasive ATR-FT-IR-spectroscopy, *Cell Mol Biol (Noisy-le-grand)*, 44, 899-912, 1998.
- Heise, HM, Non-invasive monitoring of metabolites using near infrared spectroscopy: state of the art, *Horm Metab Res*, 28, 527-534, 1996.
- Heise, HM, Technology for Non-Invasive Monitoring of Glucose, *18th Annual International Conference of the IEEE Engineering in Medicine and Biology Society* (Amsterdam), 1996.
- Hidalgo J. I., Colmenar M. J., Risco-M. J. L., Maqueda E., Botella M., Rubio J.A., Infante A.C., Garnica O., Lanchares J., Clarke and Parkes error grid analysis of diabetic glucose models obtained with evolutionary computation, In *Proceedings of the 2014 conference companion on Genetic and evolutionary computation companion (GECCO Comp '14)*, ACM, New York, NY, USA, 1305-1312, 2014.

- Hill B., Accu-Chek Advantage: Electrochemistry for Diabetes Management, *Current Separations*, 2014.
- Hillier TA, Abbott RD, Barrett EJ. Hyponatremia: evaluating the correction factor for hyperglycemia. *Am J Med.*, 106(4), 399–403, 1999.
- Huang, D, Swanson, EA, Lin, CP, Schuman, JS, Stinson, WG, Chang, W, Hee, MR, Flotte, T, Gregory, K, Puliafito, CA and et al., Optical coherence tomography, *Science*, 254,1178–1181,1991.
- Huisman TH, Martis EA, Dozy A, Chromatography of hemoglobin types on carboxymethylcellulose. *J.Lab. Clin. Med.* 52 (2): 312–327, 1958.
- Iiya Fine, Glucose correlation with light scattering patterns, Chapter 9, Valery V. Tuchin (Editor.), Handbook of Optical Sensing of Glucose in Biological Fluids and Tissues, *CRC Press, Taylor & Francis Group*,6000 Broken Sound Parkway NW, Suite 300 Boca Raton, FL 33487-2742, 237-280, 2009.
- International Diabetes Federation, IDF Diabetes Atlas, 6th edn. Brussels, Belgium: *International Diabetes Federation*, 2013. <http://www.idf.org/diabetesatlas>.
- ISO 15197. In vitro diagnostic test systems--requirements for blood glucose monitoring systems for self-testing in managing diabetes mellitus. Geneva, Switzerland: *International Organization for Standardization*; 2013.
- ISO 15197. In vitro diagnostic test systems--requirements for blood glucose monitoring systems for self-testing in managing diabetes mellitus. Geneva, Switzerland: *International Organization for Standardization*; 2006.
- ISO 15197. In vitro diagnostic test systems--requirements for blood glucose monitoring systems for self-testing in managing diabetes mellitus. Geneva, Switzerland: *International Organization for Standardization*; 2003.
- Jeckelmann, J and Seibold, A, GlucOnline - a new approach to continuous glucose monitoring, *Diabetes profile*, 2002.
- Kayashima S, Arai T, Kikuchi M, Sato N, Nagata N, Takatani O, Ito N, Kimura J, Kuriyama T, Kaneyoshi A., New noninvasive transcutaneous approach to blood glucose monitoring: successful glucose monitoring on human 75 g OGTT with novel sampling chamber, *IEEE Trans Biomed Eng.*, Aug, 38(8), 752-757, 1991.
- Kelly, JJ, Kelly, KA and Barlow, CH, Tissue temperature by near-infrared spectroscopy, *Optical Tomography, Photon Migration, and Spectroscopy of Tissue and Model Media: Theory, Human Studies, and Instrumentation* 1995, 818-828, 1995.
- Khalil OS., Non-invasive monitoring of diabetes; Specificity, compartmentalization and calibration issues, in *Advances in Fluorescence*, C. Geddes Editor, *Kulwar Publications*, 11, 157–188, 2006.
- Khalil OS., Non-invasive glucose measurement technologies: an update from 1999 to the dawn of the new millennium, *Diabetes Technology and Therapeutics*, 6(5), 660–697, 2004.

- Khalil OS., Noninvasive photonic-crystal material for sensing glucose in tears. *Clin Chem.*, 50(12), 2236–2237, 2004.
- Khalil OS., Yeh S J, Lowery M. G., et al., Temperature modulation of the visible and near infrared absorption and scattering coefficients of intact human skin, *J. Biomed. Opt.*, 8, 191–205, 2003.
- Khalil, OS., Spectroscopic and Clinical Aspects of Noninvasive Glucose Measurements, *Clin Chem*, 45, 165-177, 1999.
- Kim, YJ, Hahn, S and Yoon, G, Determination of glucose in whole blood samples by mid-infrared spectroscopy, *Appl Opt*, 42, 745-749, 2003.
- King L.V., On the acoustic radiation pressure on spheres, *Proceedings of the Royal Society of London*, A147, 212–240, 1934.
- Kinnunen M, Myllyla R. Application of optical coherence tomography, pulsed photoacoustic technique, and time-of-flight technique to detect changes in the scattering properties of a tissue-simulating phantom, *J. Biomed. Opt*, 13(2), 024005, 2008.
- Kinnunen, M and Myllyla, R, Effect of glucose on photoacoustic signals at wavelengths of 1064 and 532nm in pig blood and intralipid, *Journal of Physics D: Applied Physics*, 38, 2654-2661, 2005.
- Kinnunen, M, Myllyla, R, Jokela, T and Vainio, S, In vitro studies toward noninvasive glucose monitoring with optical coherence tomography, *Appl Opt*, 45, 2251-2260, 2006.
- Klonoff David C., Lias Courtney, Vigersky Robert, Clarke William, Parkes Joan Lee, Sacks David B., Kirkman M. Sue, Kovatchev Boris, and the Error Grid Panel, The Surveillance Error Grid, *Journal of Diabetes Science and Technology*, 1–15, 2014.
- Koenig RJ, Peterson CM, Jones RL, Saudek C, Lehrman M, Cerami A, Correlation of glucose regulation and hemoglobin A1c in diabetes mellitus, *N. Engl. J. Med.* 295 (8), 417–420, 1976.
- Kohl M., Esseupreis M., Cope M., The influence of glucose concentration upon the transport of light in tissue- simulating phantoms, *Phys. Med. Biol.*, 40, 1267-1287, 1995.
- Kohl M., M. Cope, M. Essenpreis, D. Böcker, Influence of Glucose Concentration on Light Scattering in Tissue- Simulating Phantoms, *Opt. Lett.*, 19, 2170–2172, 1994.
- Konig K., Multiphoton microscopy in life sciences, *Journal of Microscopy*, 200(2), 83-104. 2000.
- Koolman, J and Roehm, KH, *Color Atlas of Biochemistry, 2nd Edition*, Thieme, Stuttgart, New York, 35-36, 2005.
- Kost G.J, Tran N.K, Louie R.F, Gentile N, Nicole I. Gentile B.S, Abad J.V, Assessing the Performance of Handheld Glucose Testing for Critical Care, *Diabetes Technology and Therapeutics*, 10(6), 445-451, 2008.
- Krouwer JS., Why Bland-Altman plots should use X, not $(Y+X)/2$ when X is a reference method, *Statistics in Medicine*, 27, 778-780. 2008.

- Krouwer JS, Monti KL., A simple, graphical method to evaluate laboratory assays. *Eur J Clin Chem Clin Biochem*, 33, 525-527, 1995.
- Kulcu, E, Tamada, JA, Reach, G, Potts, RO and Lesho, MJ, Physiological Differences Between Interstitial Glucose and Blood Glucose Measured in Human Subjects, *Diabetes Care*, 26, 2405-2409, 2003.
- Kulkarni, O.C, Mandal, P., Das, S.S., Banerjee, S., A Feasibility study on Noninvasive Blood Glucose Measurement Using Photoacoustic Method, *4th International Conference on Bioinformatics and Biomedical Engineering (iCBBE)*, 1-4, 18-20 June, 2010.
- Kumar PR, Bhansali A, Ravikiran M, Bhansali S, Dutta P, Thakur JS, Sachdeva N, Bhadada SK, Walia R, Utility of glycated hemoglobin in diagnosing type 2 diabetes mellitus: a community-based study. *J Clin Endocrinol Metab*, 95(6), 2832–2835, 2010.
- Kurnik RT, Oliver JJ, Waterhouse SR, et al., Application of the Mixtures of Experts algorithm for signal processing in a noninvasive glucose monitoring system. *Sensors and Actuators B: Chemical.*, 60, 19-26,1999.
- Lambert, J, Storie-Lombardi, M and Borchert, M, Measurement of Physiologic Glucose Levels Using Raman Spectroscopy in a Rabbit Aqueous Humor Model, *IEEE*, 1998.
- Lam, Chak Hing., Clinical evaluation of noninvasive blood glucose measurement by using Near Infrared spectroscopy via inter and intra subject analysis, PhD Thesis, *School of Nursing, The Hong Kong Polytechnic University*, Hong Kong, 1-53, September, 2008.
- Larin K.V., Eledrisi M.S., Motamedi M., Esenaliev R.O., Noninvasive blood glucose monitoring with optical coherence tomography: a pilot study in human subjects, *Diabetes Care*, 25, 2263–2267, 2002.
- Larin K.V., Motamedi M., Ashitkov T.V., and Esenaliev R.O., Specificity of noninvasive blood glucose sensing using optical coherence tomography technique: a pilot study, *Phys. Med. Biol.*, 48, 1371–1390, 2003.
- Leboulanger, B, Guy, RH and Delgado-Charro, MB, Reverse iontophoresis for non-invasive transdermal monitoring, *Physiol Meas*, 25, R35-50, 2004.
- Lee S, Nayak V, Dodds J, Pishko M, Smith NB. Glucose measurements with sensors and ultrasound. *Ultrasound Med Biol.*, 31(7), 971–977, 2005.
- Li-Na Li, Qing-Bo Li, Guang-Jun-Zhang, A weak signal extraction method for human blood glucose noninvasive measurement using near infrared spectroscopy, *J Infrared Milli Terahz Waves*, 30, 1191-1204, 2009.
- Lipson J, Bernhardt J, Block U, Freeman W. R., Hofmeister R, Hristakeva M, B.S., Lenosky T, McNamara R, Petrasek D, Veltkamp D, and Waydo S, Requirements for Calibration in Noninvasive Glucose Monitoring by Raman Spectroscopy, *Journal of Diabetes Science and Technology*, Volume 3, Issue 2, 2009, 233-241, 2009.

- Liu, R, Chen, W, Gu, X, Wang, RK and Xu, K, Chance correlation in non-invasive glucose measurement using near-infrared spectroscopy, *Journal of Physics D: Applied Physics*, 38, 2675-2681, 2005.
- Lyandres, O, Shah, NC, Yonzon, CR and Walsh Jr., JT, Real-Time Glucose Sensing by Surface-Enhanced Raman Spectroscopy in Bovine Plasma Facilitated by a Mixed Decanethiol/Mercaptohexanol Partitiion Layer, *Analytical Chemistry*, 2005,A.F.
- MacKenzie, HA, Ashton, HS, Spiers, S, Shen, Y, Freeborn, SS, Hannigan, J, Lindberg, J and Rae, P, Advances in photoacoustic noninvasive glucose testing, *Clin Chem*, 45, 1587-1595, 1999.
- Martin, WB, Mirov, S and Venugopalan, R, Using two discrete frequencies within the middle infrared to quantitatively determine glucose in serum, *Journal of Biomedical Optics*, 7, 613-617, 2002.
- McGarraugh, G, Price, D, Schwartz, S and Weinstein, R, Physiological influences on off-finger glucose testing, *Diabetes Technol Ther*, 3, 367-376. 2001.
- Malchoff, CD, Shoukri, K, Landau, JI and Buchert, JM, A novel noninvasive blood glucose monitor, *Diabetes Care*, 25, 2268-2275, 2002.
- Marbach R. and Heise H.M., Optical diffuse reflectance accessory for measurements of skin tissue by near-infrared spectroscopy, *Applied Optics*, 34, 610–621, 1995.
- Marbach, R, Koschinsky, Th, Gries, FA and Heise, HM, Noninvasive Blood Glucose Assay by Near-Infrared Diffuse Reflectance Spectroscopy of the Human Inner Lip, *Applied Spectroscopy*, 47, 875-881, 1993.
- Maruo, K, Chin, J and Tamura, M, Noninvasive Blood Glucose Monitoring by Novel Optical Fiber Probe, *Optical Diagnostics and Sensing of Biological Fluids and Glucose and Cholesterol Monitoring II*, 2002.
- Maruo, K, Tsurugi, M, Chin, J, Ota, T, Arimoto, H and Yamada, Y, Noninvasive Blood Glucose Assay Using a Newly Developed Near-Infrared System, *Journal of Selected Topics in quantum Electronics*, 9, 322-330,2003.
- Maruo, K, Tsurugi, M, Tamura, M and Ozaki, Y, In vivo noninvasive measurement of blood glucose by near-infrared diffuse-reflectance spectroscopy, *Appl Spectrosc*, 57, 1236-1244,2003.
- McClung Melanie J., Calibration Methodology for a Microwave Non-Invasive Glucose Sensor, *Master's Thesis, Baylor University, Texas, May, 2008.*
- McCreery, RL, Raman Spectroscopy for Chemical Analysis, Chemical Analysis, (Ed. J. D. Winefordner), *John Wiley & Sons*, New York, 15, 2000.
- Meiki, V and Hanaire-Broutin, H, Indication of CGMS (Continuous Glucose Monitoring System) in the functional investigations of adult type 1 diabetic patients., *Diabetes Metab (Paris)*, 27, 618-623, 2001.
- Melikyan H, Danielyan E, Kim SW, et al. Non-invasive in vitro sensing of D-glucose in pig blood. *Med Eng Phys.*, 34(3):299–304, 2012.

- Mendelson Y., Pulse oximetry: Theory and applications for noninvasive monitoring, *Clin. Chem.*, 38, 1601–1607, 1992.
- Mohan V., Shaw, S., and Saboo, B., Current glycemc status and diabetes related complications among type 2 diabetes patients in India: Data from the A1chieve study, *Journal of Association of Physicians of India.*, 61, 12-15, 2013.
- Mohammadi B.L, Klotzbuecher T, Sigloch S, Welzel K, Goddel M, Pieber R.T, Schaupp L, In vivo evaluation of a chip based near infrared sensor for continuous glucose monitoring, *Biosensors and Bioelectronics*, 53, 99-104, 2014.
- Moran GR, Jeffrey KR, Thomas JM, Stevens JR. A dielectric analysis of liquid and glassy solid glucose/water solutions. *Carbohydr Res.*, 328(4), 573–584, 2000.
- Mukaibo, Y, Shirado, H, Konyo, M and Maeno, T, Development of a Texture Senor Emulating the Tissue Structure and Perceptual Mechanism of Human Fingers, *International Conference on Robotics and Automation* (Barcelona, Spain), 2576-2581,2005.
- Myllyla Risto, Zhao Zuomin and Kinnunen Matti, Pulsed Photoacoustic Techniques and Glucose Determination in Human Blood and Tissue, Chapter 14, Valery V. Tuchin (Editor), Handbook of Optical Sensing of Glucose in Biological Fluids and Tissues, *CRC Press, Taylor & Francis Group*,6000 Broken Sound Parkway NW, Suite 300 Boca Raton, FL 33487-2742, 419-455, 2009.
- Nafie, LA, Theory of Raman Scattering, Vol. a (Eds.: I. R. Lewis and H. G. M.Edwards), *Marcel Dekker, Inc., New York*, 1-2, 2001.
- Narasimham S., Kaila G. and Anand S, Non-invasive glucose monitoring using impedance spectroscopy, *Int. J. Biomed. Eng. Techn.*, 14, 225-232, 2014.
- Nathan, D.M., D.E. Singer, Hurxthal K, and Goodson J.D, The clinical information value of the glycosylated hemoglobin assay, *New Eng.J.Med.* 310, 341–346, 1984.
- Nightingale K. R., Palmeri M. L., Nightingale R. W., and Trahey G. E., On the feasibility of remote palpation using acoustic radiation force, *J. Acoust. Soc. Am.* 110, 625–634, 2001.
- Ozaki Y, Shinzawa H, Maruo K, In Vivo Nondestructive Measurement of Blood Glucose by Near-Infrared Diffuse-Reflectance Spectroscopy, Chapter 8, Valery V. Tuchin (Editor), Handbook of Optical Sensing of Glucose in Biological Fluids and Tissues, *CRC Press, Taylor & Francis Group*,6000 Broken Sound Parkway NW, Suite 300 Boca Raton, FL 33487-2742, 419-455, 2009.
- Ogawa M, Matsumura, Yamakoshi T, Motoi K, Yamakoshi K, A New, Noninvasive in vivo optical blood glucose measurement technique using Near Infrared Radiation (Pulse Glucometry) and a proposal for “Pulse-Hemo-photometry” Blood constituent measurements, Chapter 3, Wu, Jinglong (Editor), *Technological Advancement in Biomedicine for Healthcare Applications, IGI-Global*, 18-26, 2012.
- Oliver N. S., Toumazou C., Cass A. E. G. and Johnston D. G., Glucose sensors: a review of current and emerging technology, *Diabetic Medicine*, 26, 197–210, 2009.

- Pai P. P., Sanki P K., Satyabrata S, and Banerjee S, Modelling, Verification, and Calibration of a photo acoustics based continuous noninvasive blood glucose monitoring system, *Review of Scientific Instruments*, 86, 064901, 2015.
- Pandey Megha C., Joshi A. K., Non-Invasive Optical Blood Glucose Measurement', *International Journal of Engineering Research and Applications (IJERA)*, 3(4), 129-131, Jul-Aug, 2013.
- Parkes J.L, Slatin S.L, Pardo S, Ginsberg B.H., A new consensus error grid to evaluate the clinical significance of inaccuracies in the measurement of blood glucose, *Diabetes Care*, 23(8), 1143–1148, 2000.
- Passing H, Bablok W, A new biometrical procedure for testing the equality of measurements from two different analytical methods. Application of linear regression procedures for method comparison studies in *Clinical Chemistry, Part I. J. Clin. Chem. Clin. Biochem.* 21, 709-720, 1983.
- Perry R C, Shankar R R, Fineberg N, McGill J, Baron AD, HbA1c measurement improves the detection of type 2 diabetes in high-risk individuals with non-diagnostic levels of fasting plasma glucose: the Early Diabetes Intervention Program (EDIP). *Diabetes Care*, 24(3), 465–471, 2001.
- Pfutzner A, Caduff A, Larbig M, et al., Impact of posture and fixation technique on impedance spectroscopy used for continuous and noninvasive glucose monitoring. *Diabetes Technol Ther.*, 6, 435-441, 2004.
- Pfutzner A, Klonoff D.C, P Scott, Parkes J.L., Technical Aspects of the Parkes Error Grid, *Journal of Diabetes Science and Technology*, 7(5), 1275-1281, 2013.
- Pickering TG, Hall JE, Appel LJ, Falkner BE, Graves J, Hill MN, Jones DW, Kurtz T, Sheps SG, Roccella EJ, Recommendations for blood pressure measurement in humans and experimental animals, part 1: blood pressure measurement in humans: a statement for professionals from the Subcommittee of Professional and Public Education of the American Heart Association Council on High Blood Pressure Research, *Hypertension*, 45, 142–161, 2005.
- Pickup JC, Hussain F, Evans ND, Rolinski OJ, Birch DJ. Fluorescence-based glucose sensors. *Biosens Bioelectron.*, 20(12):2555–2565, 2005.
- Pitzer, KR, Desai, S, Dunn, T, Edelman, S, Jayalakshmi, Y, Kennedy, J, Tamada, JA and Potts, RO, Detection of hypoglycemia with the GlucoWatch biographer, *Diabetes Care*, 24, 881-885, 2001.
- Polevaya Y, Ermolina I, Schlesinger M, Ginzburg BZ, Feldman Y. Time domain dielectric spectroscopy study of human cells. II. Normal and malignant white blood cells. *Biochim Biophys Acta.*, 1419(2), 257–271, 1999.
- Qu, J and Wilson, BC, Monte Carlo modeling studies of the effect of physiological factors and other analytes on the determination of glucose concentration in vivo by near infrared optical absorption and scattering measurements, *Journal of Biomedical Optics*, 2, 319-325, 1997.
- Radel S., Brandstetter M., Lendl B., Observation of particles manipulated by ultrasound in close proximity to a cone-shaped infrared spectroscopy probe, *Ultrasonics*, 50, 240–246, 2010.

- Raghavachari, R, Introduction, Near-Infrared Applications in Biotechnology, *Marcel Dekker*, New York, 1-3, 2001.
- Rahbar S, Blumenfeld O, Ranney HM (1969). Studies of an unusual hemoglobin in patients with diabetes mellitus, *Biochem. Biophys. Res. Commun.* 36(5), 838–843, 1969.
- Ramchandani N., Heptulla A R., New technologies for diabetes: a review of the present and the future. *International Journal of Pediatric Endocrinology*, 28, 1-10, 2012.
- Rhee SY, Chon S, Koh G, et al., Clinical experience of an iontophoresis based glucose measuring system. *J Korean Med Sci*, 22, 70-73, 2007.
- Riley, MR and Crider, HM, The effect of analyte concentration range on measurement errors obtained by NIR spectroscopy, *Talanta*, 52, 473,2000.
- Robinson, MR, Eaton, RP, Haaland, DM, Koepp, GW, Thomas, EV, Stallard, BR and Robinson, PL, Noninvasive glucose monitoring in diabetic patients: a preliminary evaluation, *Clin Chem*, 38, 1618-1622, 1992.
- Rosenzweig, A, Photoacoustics and Photoacoustic Spectroscopy, Chemical Analysis, Eds.: P. J. Elving and J. D. Winefordner), *John Wiley & Sons*, New York, 1-84, 1996.
- Ruchti, TL, Thennadil, SN, Blank, TB, Lorenz, A and Monfre, SL, Noninvasive measurement of glucose through the optical properties of tissue, (*Ed. U. S. Patent*), *United States of America*, 2006, <http://www.freepatentsonline.com/6990364.html>.
- Sudheendran N, Mohamed M, Mohamed G, Tuchin V.V, Larin K.V, Assessment of tissue optical clearing as a function concentration using Optical Coherence Tomography, *Journal of Innovative Optical Health Sciences*, 03, 169, 2010.
- Sharma, J.K., Business Statistics, *Pearson Education India*, Second Edition, 454, 2012.
- Schechter, Eric, Handbook of Analysis and Its Foundations, Absolute Values, *Academic Press*, ISBN 0-12-622760-8, 259–263, 1997.
- Shcherbakov M V, Brebels A, Shcherbakova N L, Tyukov A P, Janovsky T A, and Kamaev V A., A Survey of Forecast Error Measures, *World Applied Sciences Journal (Information Technologies in Modern Industry, Education & Society)*,24, 171-176, 2013.
- Schrader, W, Meuer, P, Popp, J, Kiefer, W, Menzebach, J-U and Schrader, B, Non-invasive glucose determination in the human eye, *Journal of Molecular Structure*, 735-736, 299, 2005.
- Sieg A, Guy RH, Delgado-Charro MB, Noninvasive glucose monitoring by reverse iontophoresis in vivo: application of the internal standard concept. *Clin Chem.*, 50(8), 1383–1390, 2004.
- Siegel R.J. et al., Noninvasive Transcutaneous Low Frequency Ultrasound Enhances Thrombolysis in Peripheral and Coronary Arteries, Echocardiography; *A Jrnl. of CV Ultrasound and Allied Tech*, 18(3), 247-257, 2001.
- Sierra, JF, Galban, J and Castillo, JR, Determination of Glucose in Blood Based on the Intrinsic Fluorescence of Glucose Oxidase, *Anal. Chem.*, 69, 1471-1476, 1997.

Smith, C, Marks, A and Lieberman, M, Basic Medical Biochemistry: A Clinical Approach, *Lippincott William & Wilkins*, Philadelphia, 3-491, 2005.

So C. F., K. S Choi., Wong T. K.S, J. Chung W.Y., Recent advances in noninvasive glucose monitoring, *Medical Devices: Evidence and Research*, *Dove Press*, 5, 45-52, 2012.

Srivastava R, Jayant RD, Chaudhary A, McShane MJ. Smart Tattoo, Glucose Biosensors and Effect of Coencapsulated Anti-Inflammatory Agents. *Journal of Diabetes Science and Technology*, 5(1), 76-85, 2011.

Staveren HG V, CJM Moes, J Van Marle, SA Prahl, MJC van Gemert, "Light scattering in Intralipid-10% in the wavelength range of 400-1100 nanometers," *Applied Optics* 30, 4507-4514, 1991.

Suchkova V, Farhan N. Siddiqi, Edwin L. Carstensen, Diane Dalecki, Sally Child and Charles W. Francis, Enhancement of Fibrinolysis With 40-kHz Ultrasound, *Circulation*, 98,1030-1035,1998.

Suchkova V. N., Baggs R. B. ,Francis C. W. , Effect of 40-kHz Ultrasound on Acute Thrombotic Ischemia in a Rabbit Femoral Artery Thrombosis Model Enhancement of Thrombolysis and Improvement in Capillary Muscle Perfusion, *Circulation*, 101, 2296-2301, 2000.

Syed IA., Glycated haemoglobin; past, present, and future are we ready for the change. *J Pak Med Assoc*, 61(4), 383–388, 2011.

Se-yuen, Wave experiments using low-cost 40 kHz ultrasonic transducers, *Physical Education*, *IOP publishing Ltd.*, 38 (5), 441-446, 2003.

Tarumi, M, Shimada, M, Murakami, T, Tamura, M, Shimada, M and Yamada, Y, A Monte Carlo Simulation of NIR spectrum Changes Induced by Variations of Glucose Concentration, *Proc. SPIE*, 28-35, 2002.

Tirtariyadi Ryan, Optical Glucometer Interface-Developing a Data Collecting System for Near-Infrared Bio-sensing Applications, *Electrical & Biomedical Engineering Project Report*, *McMaster University*, Canada, 2009.

Tamada JA, Garg S, Jovanovic L, et al., Noninvasive glucose monitoring: comprehensive clinical results. *Cygnus Research Team. JAMA.*, 282, 1839-1844,1999.

Tao D, Adler A. In vivo blood characterization from bioimpedance spectroscopy of blood pooling. *IEEE Trans Instrum Meas.*, 58(11), 3831–3838, 2009.

Tenhunen J., Kopola H., Myllyla R., Non-invasive glucose measurement based on selective near infrared absorption: requirements on instrumentation and special range, *Measurement*, (24), 173–177, 1998.

Tierney, MJ, Transdermal glucose monitoring opens a new age of diabetes management, *IVD Technology*, 2003.

Tittel, FK, Richter, D and Fried, A, Mid-Infrared Laser Applications in Spectroscopy, *Appl Phys*, 89, 445-516, 2003.

- Trivelli, L.A., Ranney, H.M., Lai, H.T., Hemoglobin components in patients with diabetes mellitus, *New Eng.J.Med.*, 284, 353-357, 1971.
- Tu, AT, Raman Spectroscopy in Biology: Principles & Applications, *John Wiley & Sons*, 7-47, 1982.
- Tuchin V.V (ed.), Handbook of Optical Sensing of Glucose in Biological Fluids and Tissues, *CRC Press, Taylor & Francis Group*, London, 2009.
- Tuchin V.V (ed.), Optical Clearing in Tissues and Blood, PM 154, *SPIE Optical Engineering Press*, Bellingham, WA,107-146, 2006.
- Tura A., Advances in the development of devices for noninvasive glycemia monitoring: who will win the race?, *Nutritional Therapy and Metabolism*, 28 (1), 33–39, 2010.
- Tura A., Maran A. and Pacini G., “Non-invasive glucose monitoring: Assessment of technologies and devices according to quantitative criteria”, *Diabetes Research and Clinical Practice*, vol. 77, 16-40, 2007.
- Tura A., Noninvasive glycaemia monitoring: background, traditional findings, and novelties in the recent clinical trials, *Curr Opin Clin Nutr Metab Care*, 11, 607-612, 2008.
- Tura A, Sbrignadello S, Cianciavichia D, Pacini G, Ravazzani P. A low frequency electromagnetic sensor for indirect measurement of glucose concentration: in vitro experiments in different conductive solutions. *Sensors (Basel)*, 10(6), 5346–5358, 2010.
- Urban M. W., Fatemi M., Greenleaf J F., Modulation of ultrasound to produce multifrequency radiation force, *Acoustical Society of America*, 1228–1238, 2010.
- UK Prospective Diabetes Study Group, *Tight blood pressure control and risk of macro vascular and micro vascular complications in type 2 diabetes: UKPDS 38*, 1998.
- United Kingdom Prospective Diabetes Study (UKPDS), Diabetes Trials Unit. *Oxford University*. <https://www.dtu.ox.ac.uk/ukpds/> (Last Accessed: 21/12/2015)
- Vaddiraju S, Diane J. Burgess, Loannis Tomazos, Faquir C. Jain, and Fotios P, Technologies for Continuous Glucose Monitoring: Current Problems and Future Promises, *J Diabetes Sci Technol.*, 4(6),1540-62, 2010.
- Valgimigli F, Lucarelli F, Scuffi C, Morandi S, and Sposato I, Evaluating the Clinical Accuracy of GlucoMen®Day: A Novel Microdialysis-based Continuous Glucose Monitor, *Journal of Diabetes Science and Technology*, Volume 4, Issue 5, 1182-1192, September, 2010.
- Vashist Sandeep Kumar, Non-invasive glucose monitoring technology in diabetes management: A review. *Analytica Chimica Acta*, 750, 16– 27, 2012.
- Voigt J, Wendelken M, Driver V, Alvarez OM, Low-frequency ultrasound (20-40) kHz as an adjunctive therapy for chronic wound healing: a systematic review of the literature and meta-analysis of eight randomized controlled trials, *Int J Low Extrem Wounds*, Dec, 10(4), 2011.

- Wan, Q, Cote, GL and Brandon, DJ, Dual-wavelength polarimetry for monitoring glucose in the presence of varying birefringence, *Journal of Biomedical Optics*, 10, 024029-024021-024028, 2005.
- Ward, Electrical Engineering Science, *McGraw-Hill*, 141–142, 1971.
- Watkins P. J., ABC of Diabetes, (Fifth Edition), London: *BMJ Books*, 2003.
- Wentholt I.M.E., Hart A.A.M., Hoekstra J.B.L. and Devries J.H., How to Assess and Compare the Accuracy of Continuous Glucose Monitors? *Diabetes Technology & Therapeutics*, volume 10, number 2, 57-68, 2008.
- Weiss R, Yegorchikov Y, Shusterman A, Raz I. Noninvasive continuous glucose monitoring using Photoacoustic technology: results from the first 62 subjects. *Diabetes Technol Ther.*, 9, 68-74, 2007.
- Weinzimer SA., Pendra: the once and future noninvasive continuous glucose monitoring device? *Diabetes Technol Ther.*, 6, 442-444, 2004.
- Wild S, Roglic G, Green A, Sicree R, King H. Global prevalence of diabetes: estimates for the year 2000 and projections for 2030, *Diabetes Care*, 27(5), 1047-1053, 2004.
- Wilson D, Braunwald E Isselbacher K I, Petersdorf R G, Manin J B, Fauci A S and Root R K (ed), Harrison's Principles of Internal Medicine 12th edn., *New York: McGraw-Hill*, 1991.
- Yadav, J., Rani, A., Singh, V., Murari, B.M., "Near-infrared LED based non-invasive blood glucose sensor," *2014 International Conference on Signal Processing and Integrated Networks (SPIN)*, pp.591-594, 20-21 Feb. 2014.
- Yadav J, Rani A, Singh V, Murari B M, Prospects and limitations of non-invasive blood glucose monitoring using near-infrared spectroscopy, *Biomedical Signal Processing and Control*, 18, 214–227, 2015.
- Yamakoshi Y, Ogawa M, Tamura T, Multivariate Regression and Classification Models for Estimation of Blood Glucose Levels using a New Noninvasive Optical Measurement Technique Named “Pulse-Glucometry”, *The Open Optics Journal*, 3, 63-69, 2009.
- Yamakoshi K., Yamakoshi Y., Pulse Glucometry: A New Approach for Non-invasive Blood Glucose Measurement Using Instantaneous Differential Near Infrared Spectrophotometry, *Journal of Biomedical Optics*, 11(5), 1-11, (September/October), 2006.
- Yeh S J, Kantor S., Hanna C. F., et al., Calculated calibration models for glucose in cutaneous tissue from temperature modulation of localized reflectance measurements, *Proc. SPIE*, 5771, 166–173, 2005.
- Yeh S J, Hanna C. F., Kantor S., et al., Differences in thermal optical response between intact diabetic and nondiabetic human skin, *Proc. SPIE*, 4958, 213–224, 2003.
- Yeh S.J., Hanna C.F., Khalil O.S., Monitoring blood glucose changes in cutaneous tissue by temperature-modulated localized reflectance measurements, *Clin. Chem.*, 49, 924–934, 2003.

Yonzon C.R., Haynes C.L., Zhang X., Walsh J.T. Jr., Van Duyne R.P., A glucose biosensor based on surface-enhanced Raman scattering: improved partition layer, temporal stability, reversibility, and resistance to serum protein interference, *Anal. Chem.*, 76, 78–85, 2004.

Yoon Gilwon, Statistical Analysis for Glucose Prediction in Blood Samples by Infrared Spectroscopy, Chapter 4, Valery V. Tuchin (Editor), Handbook of Optical Sensing of Glucose in Biological Fluids and Tissues, *CRC Press, Taylor & Francis Group*, 6000 Broken Sound Parkway NW, Suite 300 Boca Raton, FL 33487-2742, 97-114, 2009.

Youcef-Toumi, K and Saptari, VA, noninvasive blood glucose analysis using near infrared absorption spectroscopy, *MIT d'Arbeloff Laboratory for Information Systems and Technology*, 1-22, 1999.

Youcef-Toumi, K and Saptari, VA, Noninvasive Blood Glucose Analysis Using Near Infrared Absorption Spectroscopy, *MIT d'Arbeloff Laboratory for Information Systems and Technology*, 1-7, 2000.

Zhao Z., Myllyl R., Photoacoustic blood glucose and skin measurement based on optical scattering effect, *Proc. SPIE*, 4707, 153–157, 2002.

Zhao, Z, Pulsed photoacoustic techniques and glucose determination in human blood and tissue, *Department of Electrical Engineering and Infotech Oulu, University of Oulu*, 101-104, 2002.

Zhao Z., Pulsed Photoacoustic Techniques and Glucose Determination in Human Blood and Tissue, Doctoral thesis, *University of Oulu, Finland*, 2002.

Zhu L., Lin J., Lin B., Li H., Noninvasive blood glucose measurement by ultrasound-modulated optical technique, *Chinese Optical Letters*, 11(2), 0217011-0217015, 2013.

Zhu L., Lin J., Lin B., Li H., New optical method for noninvasive blood glucose measurement by optical ultrasonic modulation, *Proc. SPIE 7845, Optics in Health Care and Biomedical Optics IV*, 784525, November 08, 2011.

Zilberman S, Kononenko A, Weinstein A, Gabis E, Karasin A, Improved system for noninvasive glucose monitoring at home, *EASD poster*, 932, 2009.

APPENDICES

A.I Ethical Clearance Certificate:

FACULTY OF MEDICINE
INSTITUTE OF MEDICAL SCIENCES
BANARAS HINDU UNIVERSITY

No. Dean/2011-12/ 297

Dated: 01.11.2011

Dr. Neeraj Sharma
Asstt Professor & PI
School of Biomedical Engineering
Institute of Technology
Banaras Hindu University


Dear Sir,

The Ethical Committee meeting was held on 01.11.2011 at 3.00 PM in the Chamber of Dean, IMS for ethical clearance of the MD/MS/MCH/Ph.D/synopsis/Project submitted by the following:.

Name of the Teacher – Dr. Neeraj Sharma
Project Title : Development of an optical technique based noninvasive blood glucose meter
Ethical Observation-
Remarks: The project is approved by the Ethical Committee for pilot project

This is for your information and necessary action at your end.


(B.D. BHATIA)
DEAN &
COORDINATOR

Yours sincerely,

(Dr. J.K. AGRAWAL)
CHAIRPERSON OF THE ETHICAL COMMITTEE

A.II Patient Consent Form Format:

Study Title: Development of an optical technique based non-invasive blood glucose meter

Myself.....aged.....
sex.....son/daughter/wife of.....resident
of.....
.....have read the foregoing patient information sheet. I had the opportunity to ask
questions about it and any questions that I have asked have been answered to my
satisfaction. I consent voluntarily to participate as a participant in this research. I agree to
give my personal information and obtained clinical samples for the research purpose.

Signature/ Thumb impression of the participant

Signature/ Thumb impression

Name of the participant:
Date _____
Day/month/year

1. Witness.....

Relationship with the participant:
Address:

2. Witness.....

Statement by the researcher/person taking consent

I have accurately read out the information sheet to the potential participant, and to
the best of my ability made sure that the participant understands that the following will be
done:

- 1.
- 2.

I confirm that the participant was given an opportunity to ask questions about the
study, and all the questions asked by the participant have been answered correctly and to
the best of my ability. I confirm that the individual has not been coerced into giving
consent, and the consent has been given freely and voluntarily.

Name of Researcher/person taking the consent.....

Signature of Researcher/person taking the consent.....

Date _____
Day/month/year

A.III Look-up Table for converting Peak Amplitude (mV) in FFT Domain to its corresponding Predicted (Noninvasive) Blood Glucose Levels (mg/dl):

Peak Amplitude (mV)	P-BGL (mg/dl)	Peak Amplitude (mV)	P-BGL (mg/dl)	Peak Amplitude (mV)	P-BGL (mg/dl)
7.0	70	10.9	109	14.8	148
7.1	71	11.0	110	14.9	149
7.2	72	11.1	111	15.0	150
7.3	73	11.2	112	15.1	151
7.4	74	11.3	113	15.2	152
7.5	75	11.4	114	15.3	153
7.6	76	11.5	115	15.4	154
7.7	77	11.6	116	15.5	155
7.8	78	11.7	117	15.6	156
7.9	79	11.8	118	15.7	157
8.0	80	11.9	119	15.8	158
8.1	81	12.0	120	15.9	159
8.2	82	12.1	121	16.0	160
8.3	83	12.2	122	16.1	161
8.4	84	12.3	123	16.2	162
8.5	85	12.4	124	16.3	163
8.6	86	12.5	125	16.4	164
8.7	87	12.6	126	16.5	165
8.8	88	12.7	127	16.6	166
8.9	89	12.8	128	16.7	167
9.0	90	12.9	129	16.8	168
9.1	91	13.0	130	16.9	169
9.2	92	13.1	131	17.0	170
9.3	93	13.2	132	17.1	171
9.4	94	13.3	133	17.2	172
9.5	95	13.4	134	17.3	173
9.6	96	13.5	135	17.4	174
9.7	97	13.6	136	17.5	175
9.8	98	13.7	137	17.6	176
9.9	99	13.8	138	17.7	177
10.0	100	13.9	139	17.8	178
10.1	101	14.0	140	17.9	179
10.2	102	14.1	141	18.0	180
10.3	103	14.2	142	18.1	181
10.4	104	14.3	143	18.2	182
10.5	105	14.4	144	18.3	183
10.6	106	14.5	145	18.4	184
10.7	107	14.6	146	18.5	185
10.8	108	14.7	147	18.6	186

A.III Look-up Table for converting Peak Amplitude (mV) in FFT Domain to its corresponding Predicted (Noninvasive) Blood Glucose Levels (mg/dl) [Continued]:

Peak Amplitude (mV)	P-BGL (mg/dl)	Peak Amplitude (mV)	P-BGL (mg/dl)	Peak Amplitude (mV)	P-BGL (mg/dl)
18.7	187	22.6	226	26.5	265
18.8	188	22.7	227	26.6	266
18.9	189	22.8	228	26.7	267
19.0	190	22.9	229	26.8	268
19.1	191	23.0	230	26.9	269
19.2	192	23.1	231	27.0	270
19.3	193	23.2	232	27.1	271
19.4	194	23.3	233	27.2	272
19.5	195	23.4	234	27.3	273
19.6	196	23.5	235	27.4	274
19.7	197	23.6	236	27.5	275
19.8	198	23.7	237	27.6	276
19.9	199	23.8	238	27.7	277
20.0	200	23.9	239	27.8	278
20.1	201	24.0	240	27.9	279
20.2	202	24.1	241	28.0	280
20.3	203	24.2	242	28.1	281
20.4	204	24.3	243	28.2	282
20.5	205	24.4	244	28.3	283
20.6	206	24.5	245	28.4	284
20.7	207	24.6	246	28.5	285
20.8	208	24.7	247	28.6	286
20.9	209	24.8	248	28.7	287
21.0	210	24.9	249	28.8	288
21.1	211	25.0	250	28.9	289
21.2	212	25.1	251	29.0	290
21.3	213	25.2	252	29.1	291
21.4	214	25.3	253	29.2	292
21.5	215	25.4	254	29.3	293
21.6	216	25.5	255	29.4	294
21.7	217	25.6	256	29.5	295
21.8	218	25.7	257	29.6	296
21.9	219	25.8	258	29.7	297
22.0	220	25.9	259	29.8	298
22.1	221	26.0	260	29.9	299
22.2	222	26.1	261	30.0	300
22.3	223	26.2	262	30.1	301
22.4	224	26.3	263	30.2	302
22.5	225	26.4	264	30.3	303

➤ **Published Papers in SCI (Science Citation Index) Journals:**

- **Chowdhury, M.K.,** Srivastava, A., Sharma, N., Sharma, S., ‘Noninvasive blood glucose measurement utilizing a newly designed system based on modulated ultrasound and infrared light’, *International Journal of Diabetes in Developing Countries*; **Springer**, 1-10, December 2015, DOI 10.1007/s13410-015-0459-0.
- **Chowdhury, M.K.,** Srivastava, A., Sharma, N., Sharma, S., ‘The Error Grid Analysis of invasive and indigenously developed noninvasive technique based blood glucose readings obtained from the effect of various glucose concentration sample solutions over blood glucose levels on the human subjects’, *Research Journal of Biotechnology*, Vol. 10(1), 76-84, January 2015.
- **Chowdhury, M.K.,** Srivastava, A., Sharma, N., Sharma, S., ‘Estimation of fasting Blood glucose levels by invasive and indigenously developed noninvasive technology and its correlation with the Glycated hemoglobin (HbA1c) biomarker in healthy and diabetic subjects’, *Research Journal of Biotechnology*, Vol. 9(12), 64-71, December 2014.

➤ **Published Papers in International Referred Journals:**

- **Chowdhury, M.K.,** Srivastava, A., Sharma, N., Sharma, S., ‘Error Grid Analysis of Reference and Predicted Blood Glucose Level values as obtained from the Normal and Prediabetic Human Volunteers’, *American Journal of Biomedical Engineering*, 5(1), 6-14, 2015. DOI: 10.5923/j.ajbe.20150501.02
- **Chowdhury, M.K.,** Srivastava, A., Sharma, N., Sharma, S., ‘The role of amplitude modulated ultrasonic standing waves in noninvasive blood glucose level detections’, *Advances in Bio Research*, Vol. 5 (4), 103-109, December 2014. DOI:10.15515/abr.0976-4585.5.4.103109
- **Chowdhury, M.K.,** Srivastava, A., Sharma, N., Sharma, S., ‘Five days daily sessions of noninvasive blood glucose level predictions based on amplitude modulated ultrasound and infrared technique over a healthy and diabetic subject’. *Journal of Electrical and Electronics Engineering*, Vol.5.Ver. IV, 34-41, Sep-Oct., 2014. DOI: 10.9790/1676-09543441

- **Chowdhury, M.K.**, Srivastava, A., Sharma, N., Sharma, S., 'The potential application of amplitude modulated ultrasound with Infrared Technique for blood glucose level determination in noninvasive manner'. *Biomedical and Pharmacology Journal*, Vol.7, No.1, 195-206, 2014. DOI: <http://dx.doi.org/10.13005/bpj/472>
- **Chowdhury, M.K.**, Srivastava, A., Sharma, N., Sharma, S., Neeraj Sharma, 'Prospective Analysis of Developing Noninvasive Blood Glucose Monitoring Biosensors for Diabetic Population', *Bioscience Biotechnology Research Asia*, Vol. 11(3), 1639-1647, 2014. DOI: <http://dx.doi.org/10.13005/bbra/1563>
- **Chowdhury, M.K.**, Srivastava, A., Sharma, N., Sharma, S., 'The influence of blood glucose level upon the transport of light in diabetic and non-diabetic subjects'. *International Journal of Biomedical and Advance Research*, 4(5), 306-316, 2013. DOI: 10.7439/ijbar.v4i5.357
- **Chowdhury, M.K.**, Srivastava, A., Sharma, N., Sharma, S., 'Challenges & Countermeasures in Optical Noninvasive Blood Glucose Detection', *International Journal of Innovative Research in Science, Engineering and Technology (IJIRSET)*, Vol.2, Issue 1, 324-329, Jan 2013.
- **Published Papers in International Conference:**
- **Chowdhury, M.K.**, Srivastava, A., Sharma, N., Sharma, S., 'Glycemic levels relation with blood pressure in normal and hyperglycemic subjects: Its evaluation by invasive and indigenous noninvasive glycemic level detecting technology,' 2014-International Conference on Advances in Engineering and Technology Research (ICAETR-IEEE), **IEEE Explore**, pp.1-5, 1st to 2nd August, 2014. DOI: 10.1109/ICAETR.2014.7012916.
- **Abstract Published in International/National Conferences:**
- **Chowdhury, M.K.**, Srivastava, A., Sharma, N., Sharma, S., 'A Feasibility Study on Noninvasive Blood Glucose Measurement Using Amplitude Modulated Ultrasound and Infrared Technique', The 10th International Conference and Expo on Emerging Technologies for a Smarter World, 21st and 22nd of October 2013, **CEWIT 2013, Melville Marriott, Newyork, USA.**

- **Chowdhury, M.K.**, Srivastava, A., Sharma, N., Sharma, S., ‘A significant analysis for noninvasive glucose biosensors’, National Conference on Present Scenario and Future Trends in Biomedical Engineering and Healthcare Technologies (**FTBH - 2014**), October 17-18, 2014, School of Biomedical Engineering, Indian Institute of Technology (BHU), Varanasi, India.
- **Poster Presentation:**
- **Chowdhury, M.K.**, Srivastava, A., ‘Review on Developing Noninvasive Blood Glucose Monitoring Devices’, in **CARDIABCON-2014** held on November 08-09, 2014 at HHI, Varanasi, India.
- **Patent Filed:**
- Patent application filed with title: ‘Non Invasive Blood Glucose meter based on Modulated Ultrasound & Optical Technique’. Application No.**3877/DEL/2012 A**. Country: India. Date of filing of Application: 14/12/2012. Publication Date: **18/01/2013**.
- **Accolades:**
- The CARDIABCON and Diabetes Care Organization of India honored ‘**Young Scientist Award-2013**’ at HHI, Varanasi, India.
- Our research work published in “**Hindustan Times**” Newspaper with article titled as “*Monitor your blood glucose without finger prick soon*”, volume XVIII, No.270, page no.5, Friday, 20th November 2015.

PUBLICATIONS


*Noninvasive blood glucose measurement
utilizing a newly designed system based on
modulated ultrasound and infrared light*

**Md. Koushik Chowdhury, Anuj
Srivastava, Neeraj Sharma & Shiru
Sharma**

**International Journal of Diabetes in
Developing Countries**
Incorporating Diabetes Bulletin

ISSN 0973-3930

Int J Diabetes Dev Ctries
DOI 10.1007/s13410-015-0459-0

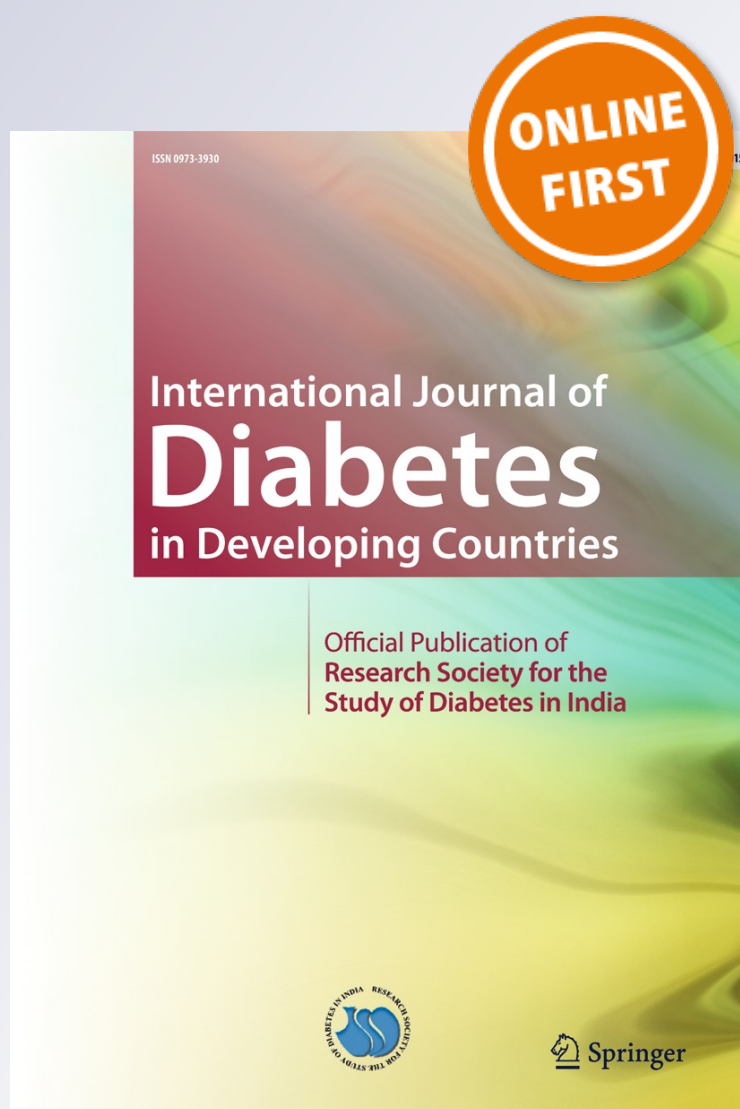

Your article is protected by copyright and all rights are held exclusively by Research Society for Study of Diabetes in India. This e-offprint is for personal use only and shall not be self-archived in electronic repositories. If you wish to self-archive your article, please use the accepted manuscript version for posting on your own website. You may further deposit the accepted manuscript version in any repository, provided it is only made publicly available 12 months after official publication or later and provided acknowledgement is given to the original source of publication and a link is inserted to the published article on Springer's website. The link must be accompanied by the following text: "The final publication is available at link.springer.com".

Noninvasive blood glucose measurement utilizing a newly designed system based on modulated ultrasound and infrared light

Md. Koushik Chowdhury¹ · Anuj Srivastava¹ · Neeraj Sharma¹ · Shiru Sharma¹

Received: 27 June 2015 / Accepted: 21 November 2015
© Research Society for Study of Diabetes in India 2015

Abstract The approach of a new noninvasive innovation for blood glucose measurement will reform management of diabetes alongside expanded patient compliance, decline load on therapeutic crisis, and diabetes associated complications. In this present work, we represent a modulated ultrasound and infrared technique-based noninvasive system for blood glucose measurement over human subjects. The oral glucose tolerance test- and random blood glucose level test-based clinical study was performed over human subjects to measure the performance of our indigenously designed system. The accuracy was examined by pairing and comparing our noninvasive predicted data with the invasive reference data. The oral glucose tolerance test and random blood glucose test produced a total of 180 and 30 paired glucose values (noninvasive vs. invasive), respectively. The root mean squared error between the noninvasive and invasive glucose value for oral glucose tolerance test and random blood glucose measurement was 23.76 mg/dl and 28.20 mg/dl, respectively. The Pearson correlation coefficient between the noninvasive and invasive glucose value for both the tests was 0.76 and 0.85, respectively. Similarly, the mean absolute error for both the tests was 15.92 mg/dl and 17.76 mg/dl, respectively. Further, the Clarke Error Grid analysis depicts that both the tests result

occupy medically accurate and acceptable zones A and B, respectively (oral glucose tolerance test: zone A=78.33 %; zone B=21.66 % and random blood glucose measurement: zone A=83.33 %; zone B=16.66 %). Hence, the present study direct towards the potentiality of our technique for noninvasive blood glucose measurement. The instrument was medically safe and well tolerated.

Keywords Oral glucose tolerance test · Random blood glucose level · Ultrasound · Infrared light · Noninvasive technique

Introduction

Diabetes has progressed as an important healthcare endemic of the contemporary world. Globally, the aggregate number of individuals with diabetes ascends from 382 million in 2013 to 592 million in 2030. Similarly, in our country (India), the total number of diabetic population increase from 65.1 million in 2013 to 109 million in 2030. Overall, the numbers of diabetics are expanding at an enormous alarming pace [1].

The diabetic subject needs to monitor blood glucose level (BGL) regularly for four to five times per day for circumventing the terminal stage medical complexities and expenses. The invasive device-based blood glucose monitoring comprises painful procedures, mental agony, and infection liabilities. For all these reasons, at present, a new noninvasive technique for blood glucose measurement is extremely demanding [2–6].

In perspective of addressing the requirement for this necessity, the present work's objective is to validate our indigenously developed noninvasive technique for blood glucose measurement in the human subjects.

✉ Md. Koushik Chowdhury
kchoudhary.rs.bme11@itbhu.ac.in

Anuj Srivastava
anuj.srivastava100@gmail.com

Neeraj Sharma
neeraj29@indiatimes.com

Shiru Sharma
shiru.bme1@gmail.in

¹ School of Biomedical Engineering, Indian Institute of Technology (Banaras Hindu University), Varanasi, Uttar Pradesh 221005, India

Literature review and our concept for noninvasive blood glucose measurement

Zhu et al. (2013) and Zhu et al. (2010) demonstrated a new hybridized technique of utilizing an ultrasound-modulated optical technique for noninvasive blood glucose measurements. Measurement of modulation depth through ultrasound-modulated scattered light produces significant in vitro results. However, their technique lacks in in vivo experiments [7, 8].

They had applied ultrasound with light modulation techniques [7, 8], but in our application, the modulated ultrasound produces vibration and the infrared light quantity, those molecule specific vibrations for noninvasive measurement of blood glucose levels in the human subjects.

When the amplitude modulating ultrasonic waves enters inside the measurement site (human finger), the blood constituent molecules undergoes vibration due to the influence of the amplitude-modulated ultrasonic waves. The pressure of the ultrasound waves generates those changes. The intrinsic properties of these molecules present in the blood medium influences the compressibility factor. The shape and size of the molecules present in the blood medium (segment) play an important role. The magnitude of influence over larger molecules is more as compared to the smaller ones [9–11].

Hence, the vibration produced in the blood medium (segment) depends on (i) its spatial arrangement, (ii) intrinsic property of the molecules and medium, and (iii) strength and frequency of the amplitude-modulated ultrasonic waves, respectively [9–11].

The pressure amplitude of the ultrasonic standing wave has maximum and minimum values twofold above the distance of a unit wavelength. Within the propagating blood tissue medium (segment), discontinuities such as blood molecules (glucose), cells achieve location-specific ultrasonic potential energy due to their presence in the respective ultrasonic zone. The suspended blood molecules (glucose) start to move and accumulate near to the zone of least ultrasonic potential energy. For blood molecules (glucose), these concentrated zones are commonly near to the pressure nodes, distanced from each other by half a wavelength space [9–11].

Now, when the molecular diameter is smaller than the wavelength of propagating ultrasound inside the measurement site, the main force of radiation (F_r) acting on the molecular volume (V_c), positioned by path of distance (z) from the pressure node, is obtained from the gradient of the molecular ultrasonic potential energy [9–11], and mathematically expressed as:

$$F_r = - \left[\frac{\pi p_0^2 V_c \beta_w}{(2\lambda)} \right] \cdot \Phi(\beta, \rho) \cdot \sin(4\pi z/\lambda) \quad (1)$$

In this present work, P_0 stands for peak amplitude of the ultrasonic pressure. (λ) denotes ultrasound wavelength in the

suspending segment. β_w signifies compressibility of the suspending segment [9–11] and mathematically expressed as:

$$\Phi(\beta, \rho) = \left[\frac{5\rho_c - 2\rho_w}{2\rho_c + \rho_w} - \left(\frac{\beta_c}{\beta_w} \right) \right] \quad (2)$$

where β_c stands for compressibility of the molecules. Notations ρ_c and ρ_w represent the respective densities of the molecules and the suspending segments, respectively [9–11].

The well-known Lambert-Beer was law applied here to measure the specific absorption (A) property of the glucose molecule at a definite light wave number (ν) and mathematically expressed as:

$$A(\nu) = -\log I(\nu)/I_0(\nu) \quad (3)$$

In this present work, the I_0 denotes the background intensity and I represents the specific light intensity at the particular wave number (ν) of actual measurements [11].

Hence, as per Urban et al. (2010) and Silva et al. (2007), we achieve the benefit of beam forming at ultrasonic frequency for localizing the radiating force energy towards the particular measurement site (human finger). It initiates the vibration phenomenon at lower frequency such that the displacements are large enough for quantification with the infrared technique, respectively [12–14].

In this present work, the signal processing toolbox of MATLAB performs observed signal analysis in Fast Fourier Transform (FFT) domain to extract blood glucose level-related embedded information. The peak voltage amplitude variations in FFT domain serves as the functional indicator for measuring actual blood glucose level in study subjects. Hence, this principle aspect forms the basis of our noninvasive blood glucose measurement.

Our noninvasive technique-based system descriptions

Initially, it includes the description regarding ultrasound transducer and light wavelength selection criteria followed by the explanation of the indigenously designed system.

Ultrasound frequency selection

Ultrasonic transducers have found numerous applications in household appliances, medical fields, industries, and oceanography [15, 16]. In the biomedical field, the 40-kHz piezoelectric-based ultrasonic transducers aids in enhancing fibrinolysis [17], tissue penetration [17, 18], clot dissolution [18, 19], thrombolysis [19], and wound healing therapy [20]. In this present work, we have selected 40-kHz central frequency-based ultrasonic transmitters for providing modulated ultrasonic waves to the measurement site (fingertip). Further, (i)

easy availability, (ii) medically safe and tolerable [15–20], (iii) less tissue heating [16–20], (iv) high skin tissue penetration [15–20], and (v) low costs of 40-kHz ultrasonic transducers have boosted our motivation for its selection.

Light wavelength selection

The composition of human blood is complex and constitutes numerous components in it. Further, glucose molecules exhibit very weak signals. The wavelength selection needs careful and well-judged approaches to overcome this particular phenomenon [21].

Kulkarni et al. [2010] and Konig [2004] described that the region extending from 600 to 1100 nm is the “Tissue Optical Window” of the living biological tissues.

The absorption spectrum of oxyhemoglobin and deoxyhemoglobin is comparatively low within the spectral wavelength band 900 to 1000 nm, respectively. The blood oxygenations vary blood optical absorption properties [22–27].

Khalil [2004] and Khalil [1999] presented that glucose molecules exhibit absorption peaks at the 939-nm (very near to 940 nm) NIR spectral band. So, considering wavelength bands within the “Tissue Optical Window” where water, oxyhemoglobin, deoxyhemoglobin exhibit low absorption profiles and good absorption properties from glucose molecules will be better to avoid any particular noise interferences [26, 27].

Further, for significant wavelength selection, we have performed glucose specificity and sensitivity analysis. The specificity refers here to the particular light wavelength where glucose exhibits maximum absorption peak characteristics. Similarly, the sensitivity refers here to the ability of the particular light wavelength to respond in accordance with the effective variations in the glucose concentration levels.

Glucose specificity analysis

To determine the maximum wavelength specificity of glucose molecule in distilled water between the 900 and 980 nm wavelength domain, we have prepared a stock solution of 2500 mg dextrose (glucose) per 10 ml of distilled water. From that prepared concentration (w/v) stock solution, 2 ml of glucose in distilled water solution has been pipetted out, poured inside the cuvette. The Digital Spectrometer Model 305 of M.S Electronics (India) is used in this present work to measure absorbance (in arbitrary unit=au) of glucose in distilled water solution. Figure 1 depicts the absorption spectra of the glucose in distilled water. Figure 1 reveals that at 940 nm, the glucose in distilled water exhibits maximum absorption peak characteristics within the infrared spectral domain of 900 to 980 nm, respectively. Further, glucose molecule exhibits absorption peak characteristics at 939 nm (very close to 940 nm) due to possible stretch and vibration of the second O-H overtone band in its molecular structure [25, 26].

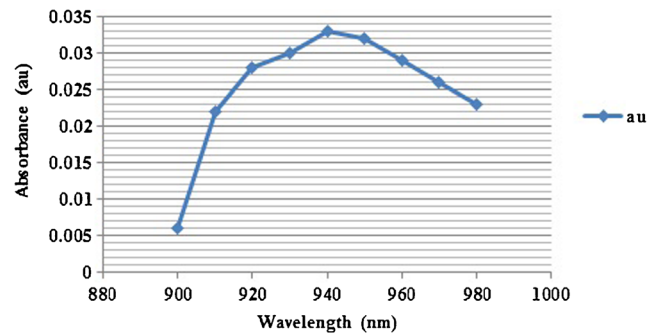


Fig. 1 Absorption spectra of glucose in distill water between 900 and 980 nm

Glucose sensitivity analysis at 940 nm

To determine the 940-nm wavelength degree of sensitivity for respective change in glucose concentration, we have prepared three sample concentration (w/v) solutions (dextrose in distilled water) like 2500 mg/10 ml, 5000 mg/10 ml, and 7500 mg/10 ml, respectively.

The Digital Spectrometer Model 305 of M.S Electronics (India) performs the measurement analysis here. Table 1 depicts the output data from those three prepared sample concentration (w/v) solutions for glucose sensitivity analysis at a 940-nm wavelength. The output data in absorbance (au) and concentration (parts per million=ppm) presents that the 940-nm wavelength has been sensitive and linearly detects the respective variations of glucose concentration (w/v) in the prepared sample solutions.

Hence, various factors like (i) “Tissue Optical Window” range (600 to 1100 nm) [21, 22], (ii) typical peak characteristic of the glucose molecule at 940 nm [21–27], (iii) acceptable specificity cum sensitivity for glucose at 940 nm [21–27], (iv) easy commercial availability [15], and (v) several literatures [28–35] favoring 940 nm for noninvasive blood glucose measurement strongly influenced us for this particular wavelength selection.

Experimental setup

In this pilot study, we have utilized the modulated ultrasound and infrared light technique-based system. The ultrasonic transmitter and receiver operate at the frequency of 40.0 ± 1.0 kHz. It can resist utmost input voltage of $20 V_{rms}$ and

Table 1 Glucose sensitivity analysis at 940 nm wavelength

Wavelength (nm)	2 ml from the prepared sample solutions (w/v)	Absorbance (au)	Concentration (ppm)
940	2500 mg/10 ml	0.033	071
	5000 mg/10 ml	0.045	113
	7500 mg/10 ml	0.067	150

produces a sound pressure output of 110 ± 5 dB at 10 V and 30 cm. In this present work, we have utilized the 940-nm infrared light emitting diode (B5B-940-8) of Roithner LaserTechnik, Vienna, Austria, for irradiating the fingertip of the study subjects. It is a round type with a 5-mm diameter, works with GaAlAs/GaAs technology, and possesses radiated output power (P_o) of 32 to 48 mW. Similarly, we have utilized EPD-1300-5.3, InGaAs selective photodiode of Roithner LaserTechnik, Vienna, Austria, for capturing transmitted light from the infrared light (940 nm)-irradiated human finger to measure noninvasive blood glucose levels. This photodiode is perfect for detection of pulsed light with sensitivity starting from 800 to 1750 nm. Figure 2 represents the block diagram of our experimental system utilized in this pilot study.

In this system as depicted in Fig. 2, the carrier wave and the modulating signal unit provides two types of typical sine wave inputs for producing the amplitude-modulated signal waves. This modulated signal serves as an input to the ultrasonic transmitter to provide the amplitude-modulated ultrasonic signal waves to the finger (measurement site) through the finger holder. Here, the ultrasonic receiver unit monitors the characteristics of the generated modulated ultrasonic waves. The modulated ultrasonic wave direction of propagation and the light source point of focus are geometrically perpendicular to the finger-positioning angle. The infrared light focused to the ultrasonic zone of impact produces output as the amplitude-modulated ultrasound light signals. The infrared detector sensitive in the infrared region acquires those specific output signals. The signal amplifier block amplifies the acquired signals. Afterwards, acquired signals were stored in the computer for

further processing through the signal processing toolbox of MATLAB to predict and display the noninvasive blood glucose levels.

Calibration

The calibration of our experimental system depends upon the peak voltage amplitude (mV) in the FFT domain corresponding to the blood glucose concentration. The calibration factor multiplies with the peak voltage amplitude (mV) in the FFT domain to provide predicted (noninvasive) blood glucose levels in milligram/deciliter and mathematically expressed as:

$$V_{\text{peak}} \times CF = \text{PBGL} \quad (4)$$

where V_{peak} stands for peak voltage amplitude (mV) in the FFT domain, CF stands for calibration factor, and PBGL refers to predicted blood glucose level in milligram/deciliter.

In vitro experiment

In order to establish a noninvasive blood glucose measurement technique, in vitro quasi-finger system (optical tissue phantoms)-based experiments are highly significant. Optical phantoms resemble tissue optical properties, in which various elementary principles and scientific concepts are tested [36–38].

In this present work, our initial approach includes preparing the quasi-finger system to mimic finger absorption and scattering characteristics in the infrared spectral domain. The

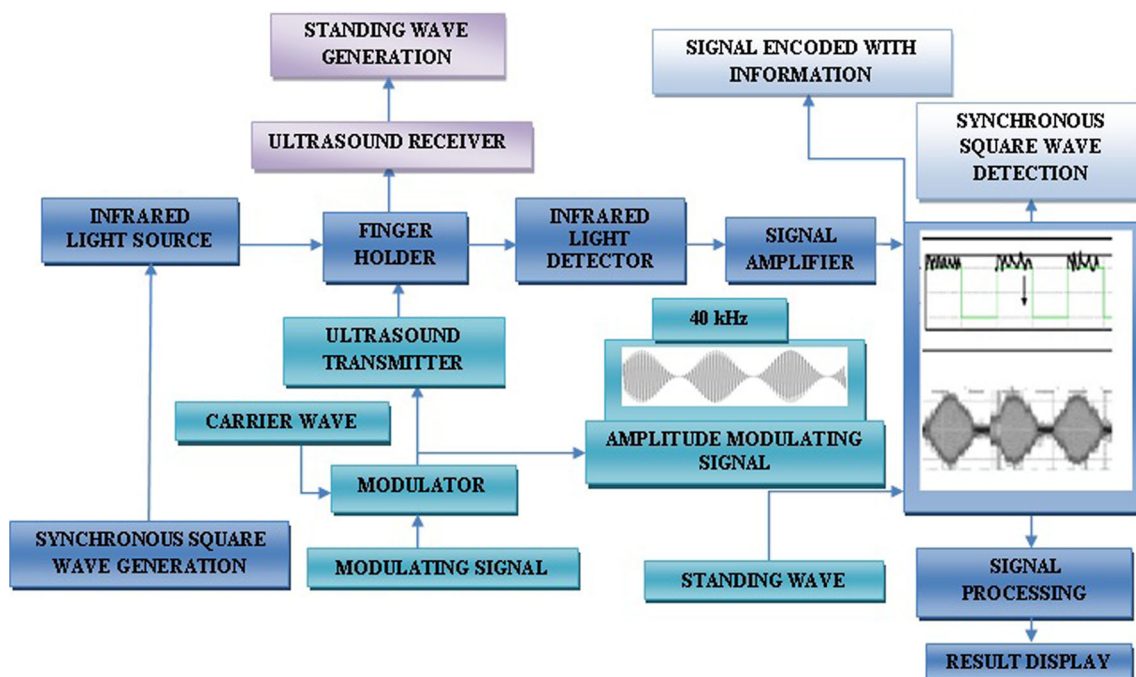


Fig. 2 Noninvasive technique-based blood glucose measuring system

intralipid phantom resembles tissue scattering aspects, while absorption is accounted here by direct addition of the whole blood samples (fasting and postprandial) to it to form the quasi-finger system [36–38].

Mixture of both of these constituents resembles blood tissue medium. The constant level of oxygen in prepared samples is essential to obtain glucose concentration-derived results [36–38].

Herein, *in vitro* (with this prepared quasi-finger system) phantom sample analysis was performed, to explore the glucose sensitivity of our noninvasive technique-based prototype unit.

Study subjects

In total, 12 adult subjects participated in this pilot study. Two subjects are healthy normal, three subjects had prediabetes, and seven subjects had diabetes. The mean±standard deviations of age is 41±5 years old and mean±standard deviations of body mass index is 27.3±3 kg/m². Overall, ten subjects were male and two subjects were female. The pilot study reported here is in accordance with the standard ethical procedures and performed with the informed consent of all the respective subjects. The pilot study was approved by the Ethical Committee Board of Faculty of Medicine, Institute of Medical Sciences, Banaras Hindu University, Varanasi, India.

Sample preparation

The sample preparation steps include:

- Step 1: Collection of whole blood samples in vacuum-based blood collecting vials, where K₂ EDTA (ethylene diamine tetra acetic acid) is present as an anticlotting agent. Addition of phosphate buffer solution (PBS) to maintain the pH levels in the samples
- Step 2: De-oxygenation of the whole blood samples by nitrogen gas bubbling for 45 min to reduce oxygen influence over glucose measurement
- Step 3: One milliliter of the intralipid suspension mixed with 1 ml of whole blood sample to form a quasi-finger system resembling blood tissue optical properties
- Step 4: Placing each prepared phantom samples inside the sample holder of our prototype unit for its respective glucose concentration measurement

The invasive measurements were performed to measure and compare the blood glucose levels with the FFT domain-based peak voltage amplitude (mV).

Table 2 represents the voltage amplitude in the FFT domain during fasting stage and its effective correlation with the invasive blood glucose levels. Similarly, Table 3 represents the voltage amplitude in the FFT domain during postprandial

Table 2 *In vitro* glucose sensitivity in phantom samples of fasting stage

Study subject	Invasive fasting blood glucose level (mg/dl)	Peak voltage amplitude (mV) in the FFT domain during fasting stage
Healthy subject 1	87	8.9
Healthy subject 2	89	9.2
Prediabetic subject 3	124	12.9
Prediabetic subject 4	113	11.6
Prediabetic subject 5	119	12.3
Diabetic subject 6	179	18.3
Diabetic subject 7	221	23.8
Diabetic subject 8	168	17.8
Diabetic subject 9	171	16.6
Diabetic subject 10	164	17.2
Diabetic subject 11	201	19.8
Diabetic subject 12	233	22.7

stage and its effective correlation with the invasive blood glucose levels.

In both Tables 2 and 3, the voltage amplitude in the FFT domain changes in correlation with the variation of invasive blood glucose levels.

These correlated changes indicate towards the sensitivity (at 940 nm) of our prototype unit in detecting glucose concentration variations in respective quasi-finger system based *in vitro* samples.

Further, voltage amplitude in the FFT domain increases with increase in blood glucose levels, this phenomenon indicates towards the glucose concentration-induced light clearing

Table 3 *In vitro* glucose sensitivity in phantom samples of postprandial stage

Study subject	Invasive postprandial blood glucose level (mg/dl)	Peak voltage amplitude (mV) in the FFT domain during postprandial stage
Healthy subject 1	103	10.5
Healthy subject 2	109	11.3
Prediabetic subject 3	159	16.5
Prediabetic subject 4	164	17.2
Prediabetic subject 5	153	15.8
Diabetic subject 6	261	25.9
Diabetic subject 7	311	31.9
Diabetic subject 8	307	32.2
Diabetic subject 9	272	28.9
Diabetic subject 10	291	30.8
Diabetic subject 11	288	31.5
Diabetic subject 12	301	33.7

effects. As increase in glucose concentration in vitro samples causes reduction of the scattering effects, which minimizes the mismatch of the refractive index acquiescently, increase in light transmission occurs [36–38].

The effective correlation in vitro experiment forms the benchmark as well as foundation for performing in vivo experiments to establish the performance and efficacy of our technique in blood glucose measurement.

In vivo experiment

Study subjects

In total, 60 adult subjects participated in this pilot study, out of which, 30 healthy adult subjects participated for OGTT analysis. Next, 30 adult subjects participated for random blood glucose level tests. Eighteen subjects are healthy normal, seven subjects had prediabetes, and five subjects had diabetes. All the prediabetic and diabetic subjects followed their normal routine of meal intake and medications. The mean±standard deviations of age is 40±4 years old and mean±standard deviations of body mass index is 26.2±2 kg/m². Overall, 44 subjects were male and 16 subjects were female. The pilot study reported here is in accordance with the standard ethical procedures and performed with the informed consent of all the respective subjects. The pilot study was approved by the Ethical Committee Board of Faculty of Medicine, Institute of Medical Sciences, Banaras Hindu University; Varanasi, India.

Experimental protocol

In this present work, the pilot study consists of two phases (oral glucose tolerance test and random test) to validate the clinical correlation between the invasive technique- and non-invasive technique-based blood glucose levels.

During the first phase, we have performed oral glucose tolerance tests over healthy subjects after their overnight fasting. The duration of each experiment was 2 h and 45 min (10 to 15 min for baseline observation before intake of 75-g glucose solution). The invasive and noninvasive data were recorded every 30 min from the right and left-hand fingers, respectively.

The Accu Chek Active of Roche Diagnostics, Germany [39] and our technique-based system performed reference (invasive) and predicted (noninvasive) blood glucose measurement here, respectively.

Throughout the investigation, the study subjects remain static to reduce motion artifacts and intake of any food or liquids were restricted.

During the second phase, we have performed random blood glucose level analysis (both invasive and noninvasive) over normal, prediabetic, and diabetic subjects, respectively.

Result and discussion

In this present work, for result analysis, we have performed Clarke error analysis and statistical analysis.

The Clarke error grid analysis critically evaluates the medical importance of the differences between noninvasive (predicted) and invasive (reference) blood glucose measurements.

The Clarke Error Grid analysis has been the universal approach for evaluating medical significance of the developing glucose sensor (mostly noninvasive)-based techniques for blood glucose determination.

The Clarke Error Grid consist of five different zones in the XY-Cartesian graph with the following interpretations: Zone A: medically accurate, Zone B: medically significant and tolerable, and Zone C to E: medically insignificant and dangerous. Further, the diagonal line where $X=Y$, expresses the ideal measurements. The data points below and above the diagonal line represent the overestimation and underestimation of the real blood glucose values, respectively. When any data pair points fall over the borderline of any zones, the nearness of its (X, Y) coordinate towards either zone determines its zone of occupancy [40–46].

Figure 3 depicts the Clarke Error Grid analysis of the oral glucose tolerance test (180 data pairs)-based BGL data measured by our noninvasive system in comparison to the BGL data measured by invasive device (Accu Chek Active of Roche Diagnostics, Germany).

The Clarke Error Grid analysis presents as follows: A zone=78.33 % and B zone=21.66 %, and none of the values in C to E zones. Hence, oral glucose tolerance test yields that all the noninvasive blood glucose readings occupy A and B zones which are medically important and acceptable.

Table 4 represents invasive and noninvasive blood glucose levels as measured during random blood glucose tests in over 30 study subjects. Figure 4 represents the Clarke Error Grid

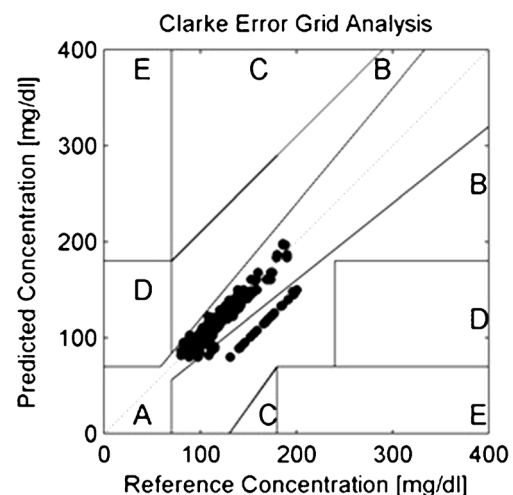


Fig. 3 Clarke Error Analysis of blood glucose data as measured during oral glucose tolerance tests

analysis of the random blood glucose measurement. The Clarke Error Grid Analysis depicts that all the measurements occupy A and B zones (Zone A=83.33 %, Zone B=16.66 %).

Hence, the random blood glucose measurement represents that all the noninvasive readings are medically significant and acceptable.

Now, the statistical analysis applied here evaluates the blood glucose levels measuring accuracy of our noninvasive technique-based prototype unit during oral glucose tolerance test and random blood glucose measurements.

Table 5 represents the mathematical expressions of the accuracy measure parameters utilized in this present work over the N number of total samples. All these accuracy measure evaluates the correctness of predicted noninvasive blood glucose levels with respect to the reference invasive blood glucose levels.

Table 4 Invasive and noninvasive blood glucose levels measured during random blood glucose tests

Subjects	Reference (invasive) BGL (mg/dl)	Predicted (noninvasive) BGL (mg/dl)
01	105	98
02	153	146
03	98	116
04	130	122
05	302	263
06	118	124
07	181	172
08	126	119
09	148	140
10	133	127
11	136	129
12	184	241
13	110	117
14	113	106
15	198	147
16	132	123
17	140	133
18	220	225
19	110	115
20	204	141
21	106	101
22	130	122
23	239	246
24	117	111
25	298	203
26	160	154
27	103	114
28	129	138
29	187	231
30	99	108

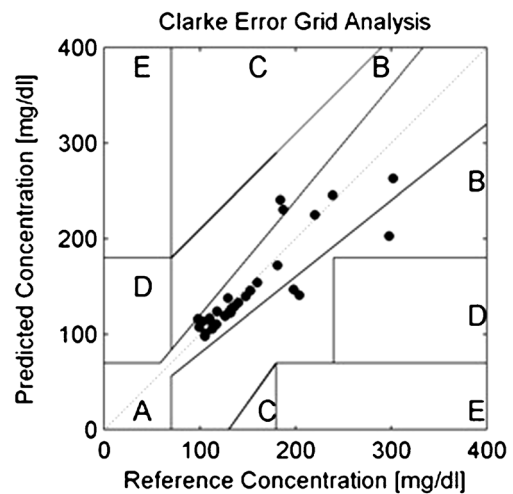


Fig. 4 Clarke Error Analysis of blood glucose data as measured during random blood glucose measurements

Table 6 depicts the statistical analysis-based summary of invasive vs. noninvasive accuracy measures obtained during the pilot study over study subjects. The performance metrics-based errors MAE, MSE, and RMSE values range from 15.92 mg/dl to 17.76 mg/dl, 564.78 mg²/dl² to 795.76 mg²/dl², and 23.76 mg/dl to 28.20 mg/dl, respectively. The performance metrics-based relative errors MARE, MSRE, and RMSRE values range from 0.11 mg/dl/min to 0.10 mg/dl/min, 0.02 mg²/dl²/min² to 0.01 mg²/dl²/min², and 0.15 mg/dl/min to 0.13 mg/dl/min, respectively. Similarly, the performance metrics-based percentage errors MAPE, MSPE, and RMSPE values range from 11.09 % to 10.10 %, 232.48 % squared to 181.40 % squared, and 15.24 % to 13.46 %, respectively. Further, the correlation coefficient (R value) value ranges from 0.76 to 0.85 respectively.

Table 6 depicts that our root mean square error (RMSE) for oral glucose tolerance test and random blood glucose measurement was 23.76 mg/dl and 28.20 mg/dl, respectively. These values are significantly comparable with other noninvasive technique-based ranges that extend from 25 to 46 mg/dl [46, 51, 52].

Further, Table 6 depicts the R value (Pearson correlation coefficient) for oral glucose tolerance test and random blood glucose measurement was 0.76 and 0.85, respectively. These values are important and comparable with the R value (correlation coefficient) of various other in vivo non-invasive techniques, which extends from 0.49 to 0.95 [51, 52], respectively.

From the perspective of the Clarke and Error Grid analysis, all the noninvasive readings occupy medically significant zones (A and B) and none of the measurements occupy medically insignificant zones (C–E).

Hence, all the overlaid findings including in vitro analysis, Clarke error grid analysis, and performance metrics-based

Table 5 Accuracy measure parameters

Accuracy measure	Mathematical expression	Symbol notations	References
MAE (mean absolute error)	$\frac{\sum_{i=1}^N y_i - \hat{y}_i }{N}$	Where y_i is the reference blood glucose level (RBGL), \hat{y}_i is the predicted blood glucose level (PBGL), and N represents the total number of samples	[47–49]
MSE (mean squared error)	$\frac{\sum_{i=1}^N (y_i - \hat{y}_i)^2}{N}$		
RMSE (root mean squared error)	$\sqrt{\frac{\sum_{i=1}^N (y_i - \hat{y}_i)^2}{N}}$		
MARE (mean absolute relative error)	$\frac{\sum_{i=1}^N \left \frac{y_i - \hat{y}_i}{y_i} \right }{N}$		
MSRE (mean squared relative error)	$\frac{\sum_{i=1}^N \left(\frac{y_i - \hat{y}_i}{y_i} \right)^2}{N}$		
RMSRE (root mean squared relative error)	$\sqrt{\frac{\sum_{i=1}^N \left(\frac{y_i - \hat{y}_i}{y_i} \right)^2}{N}}$		
MAPE (mean absolute percentage error)	$\frac{\sum_{i=1}^N \left \frac{y_i - \hat{y}_i}{y_i} \right \times 100}{N}$		
MSPE (mean squared percentage error)	$\frac{\sum_{i=1}^N \left[\left(\frac{y_i - \hat{y}_i}{y_i} \right) \times 100 \right]^2}{N}$		
RMSPE (root mean squared percentage error)	$\sqrt{\frac{\sum_{i=1}^N \left[\left(\frac{y_i - \hat{y}_i}{y_i} \right) \times 100 \right]^2}{N}}$		
Pearson correlation coefficient (R value)	$\frac{N(\sum xy) - (\sum x)(\sum y)}{\sqrt{[N\sum x^2 - (\sum x)^2][N\sum y^2 - (\sum y)^2]}}$	Where x represents RBGL value, y represents PBGL value, and N represents total number of samples.	[50]

Table 6 The accuracy measurement summary of OGTT and random blood glucose measurement

Statistic function (unit)	Accuracy measurement	
	Oral glucose tolerance test	Random blood glucose measurement
MAE (mg/dl)	15.92	17.76
MSE (mg ² /dl ²)	564.78	795.76
RMSE (mg/dl)	23.76	28.20
MARE (mg/dl/min)	0.11	0.10
MSRE (mg ² /dl ² /min ²)	0.02	0.01
RMSRE (mg/dl/min)	0.15	0.13
MAPE (%)	11.09	10.10
MSPE (% squared)	232.48	181.40
RMSPE (%)	15.24	13.46
R value	0.76	0.85

accuracy analysis depict the strong promising aspect of our noninvasive technique for blood glucose measurement in the human subjects.

However, certain error-induced bio-signals were observed due to multiple superfluous causes such as finger placement, finger shape and size, motion artifacts, time and machine drift issues, melanin-induced skin pigmentations, variation in multiple physiological parameters (blood pressure, heart rate, skin sweating, body temperature), and environmental changes, which changes blood tissue optical characteristics and induce variations in the signal acquisition processes. In future works, acquiring preventive measures is essential to reduce the abovementioned interferences.

Conclusion

We have represented the indigenously designed modulated ultrasound and infrared technique-based system for

noninvasive blood glucose measurement on human subjects. Both the in vitro and in vivo results showed good correlation in glucose measurements.

Further, the result of the Clarke error grid analysis and statistical evaluations values validates that our noninvasive system is potentially capable in performing noninvasive blood glucose measurement over human subjects.

Our noninvasive system was medically safe, easy, and acceptable, as reflected by the overall study subject's well-tolerated compliances.

Therefore, a new technique for noninvasive blood glucose measurement using modulated ultrasound and infrared technique is developed and the observation validates the supposition of the new concept. Positively, our technique will show its functional usage in the future for noninvasive estimations of blood glucose levels in human subjects.

Acknowledgments All the authors of the manuscript wish to thank the Coordinator and other faculty members of the School of Biomedical Engineering, IIT-(BHU), Varanasi, for their support throughout the experimental and the manuscript preparation procedures. Further, the corresponding author wishes to thank the MHRD (Ministry of Human Resource Development) and IIT (BHU), Varanasi, for providing him Teaching Assistantship (TA-ship) to pursue his Doctoral Degree.

Authors' contribution Md. Koushik Chowdhury, the Doctoral student, wrote the manuscript and is the corresponding author of the manuscript. Md. Koushik Chowdhury and Anuj Srivastava performed experimentations and data collection during the studies. Dr. Neeraj Sharma (associate professor) and Dr. Shiru Sharma (assistant professor) helped in overall supervision for the experimentations, final editing of the manuscript, and getting the necessary formal applications required for the experimental purposes.

Compliance with ethical standards

Conflict of interest The authors declare that they have no competing interests.

Research involving human participants and/or animals-ethical approval All procedures performed in studies involving human participants were in accordance with the ethical standards of the institutional and/or national research committee and with the 1964 Helsinki Declaration and its later amendments or comparable ethical standards. This article does not contain any studies with animals performed by any of the authors.

Informed consent Informed consent was obtained from all individual participants included in the study.

References

1. International Diabetes Federation. IDF diabetes atlas. 6th ed. Brussels: International diabetes Federation; 2013. <http://www.idf.org/diabetesatlas>. (23/05/2015).
2. So C. F., K. S. Choi., Wong T. K.S, J. Chung W.Y. Recent advances in noninvasive glucose monitoring, *Medical Devices: Evidence and Research*, Dove Press, 2012; 5: 45–52.
3. Maruo K, Tsurugi M, Chin J, Ota T, Arimoto H, Yamada Y. Noninvasive blood glucose assay using a newly developed near-infrared system. *IEEE J Sel Top Quantum Electron*. 2003;9:322–30.
4. Tuchin VV, editor. *Handbook of optical sensing of glucose in biological fluids and tissues*. London: CRC Press. Taylor & Francis Group; 2009.
5. Tura A, Maran, Pacini G. Non-invasive glucose monitoring: assessment of technologies and devices according to quantitative criteria. *Diabetes Res Clin Pract*. 2007;77:16–40.
6. Tura A. Advances in the development of devices for noninvasive glycemia monitoring: who will win the race? *Nutritional Therapy and Metabolism*. 2010;28(1):33–9.
7. Zhu L, Lin J, Lin B, Li H. Noninvasive blood glucose measurement by ultrasound-modulated optical technique. *Chin Opt Lett*. 2013;11(2):0217011–5.
8. Zhu Lili, Lin Jieqing, Xie Wenming, Hui Li. New optical method for noninvasive blood glucose measurement by optical ultrasonic modulation, *Proc. SPIE 7845, Optics in Health Care and Biomedical Optics IV*. 2010;784525.
9. Coakley WT. Ultrasonic separations in analytical biotechnology. *Trends Biotechnol*. 1997;15:506–11.
10. Haar TG, Wyard SJ. Blood cell banding in ultrasonic standing wave fields: a physical analysis. *Ultrasound Med Biol*. 1978;4(2):111–23.
11. Radel S, Brandstetter M, Lendl B. Observation of particles manipulated by ultrasound in close proximity to a cone-shaped infrared spectroscopy probe. *Ultrasonics*. 2010;50:240–6.
12. Silva GT, Urban MW, Fatemi M. Multifrequency radiation force of acoustic waves in fluids. *Physica D*. 2007;232:48–53.
13. Urban MW, Fatemi M, Greenleaf JF. Modulation of ultrasound to produce multifrequency radiation force. *Acoustical Society of America*, 2010; 1228–38.
14. Urban MW, Silva GT, Fatemi M, Greenleaf JF. Multifrequency vibro acoustography. *IEEE Trans Med Imaging*. 2006;25:1284–95.
15. Mak S.Y., Wave experiments using low-cost 40 kHz ultrasonic transducers, *Physical Education*, IOP publishing Ltd. 2003; 38 (5): 441–46.
16. Greenslade TB. Experiments with ultrasonic transducers. *Phys Teach*. 1994;32:392–7.
17. Suchkova V, Farhan N, Siddiqi AA, Carstensen EL, Dalecki D, Sally C, et al. Enhancement of fibrinolysis with 40-kHz ultrasound. *Circulation*. 1998;98:1030–5.
18. Birnbaum Y, Luo H, Nagai T, Fishbein MC, Peterson TM, Li S, et al. Noninvasive in vivo clot dissolution without a thrombolytic drug recanalization of thrombosed iliofemoral arteries by transcatheter ultrasound combined with intravenous infusion of microbubbles. *Circulation*. 1998;97:130–4.
19. Suchkova VN, Baggs RB, Francis CW. Effect of 40-kHz ultrasound on acute thrombotic ischemia in a rabbit femoral artery thrombosis model enhancement of thrombolysis and improvement in capillary muscle perfusion. *Circulation*. 2000;101:2296–301.
20. Voigt J, Wendelken M, Driver V, Alvarez OM. Low-frequency ultrasound (20–40) kHz as an adjunctive therapy for chronic wound healing: a systematic review of the literature and meta-analysis of eight randomized controlled trials. *Int J Low Extrem Wounds*. 2012;11(1):69.
21. Tenhunen J, Kopola H, Myllyla R. Non-invasive glucose measurement based on selective near infrared absorption: requirements on instrumentation and special range. *Measurement*. 1998;24:173–7.
22. Kulkarni OC, Mandal P, Das SS, Banerjee S. A feasibility study on noninvasive blood glucose measurement using photoacoustic method. 4th International Conference on Bioinformatics and Biomedical Engineering (iCBBE). 2010; 1–4.

23. König K. Multiphoton microscopy in life sciences. *J Microsc.* 2004;200(2):83–104.
24. Van Assendelft OW, editors. Spectrophotometry of hemoglobin derivatives. Assen: Royal Van Gorcum Ltd; 1970.
25. Mendelson Y. Pulse oximetry: theory and applications for noninvasive monitoring. *Clin Chem.* 1992;38:1601–7.
26. Khalil OS. Non-invasive glucose measurement technologies: an update from 1999 to the dawn of the new millennium. *Diabetes Technol Ther.* 2004;6(5):660–97.
27. Khalil OS. Spectroscopic and clinical aspects of noninvasive glucose measurements. *Clin Chem.* 1999;45:165–77.
28. McEwen MP, Reynolds KJ. Noninvasive monitoring with strongly absorbed light. *Opt Appl.* 2014;XLIV(2):177–90.
29. Bin Zainul, Abidin MT, Rosli MKR, Shamsuddin SA, Madzhi NK, Abdullah MF. Initial quantitative comparison of 940nm and 950nm infrared sensor performance for measuring glucose non-invasively. 2013 I.E. International Conference on Smart Instrumentation, Measurement and Applications (ICSIMA). 2013; 1–6.
30. Kumar VS. Non-invasive glucose monitoring technology in diabetes management: a review. *Anal Chim Acta.* 2012;75:16–27.
31. Cohen O, Fine I, Monashkin E, Karasik A. Glucose correlation with light scattering patterns—a novel method for non-invasive glucose measurements. *Diabetes Technol Ther.* 2003;5:11–7.
32. Pandey MC, Joshi AK. Non-invasive optical blood glucose measurement. *International Journal of Engineering Research and Applications (IJERA).* 2013;3(4):129–31.
33. Iiya F. Glucose correlation with light scattering patterns. Chapter 9. In: Tuchin VV, editor. *Handbook of optical sensing of glucose in biological fluids and tissues.* London: CRC Press, Taylor & Francis Group; 2009.
34. Tirtariyadi R. Optical glucometer interface-developing a data collecting system for near-infrared bio-sensing applications. *Electrical & biomedical engineering project report.* Canada: McMaster University; 2009.
35. Yadav J, Rani A, Singh V, Murari BM. Near-infrared LED based non-invasive blood glucose sensor. 2014 International Conference on Signal Processing and Integrated Networks (SPIN). 2014; 591–594.
36. Amir O, Weinstein D, Zilberman S, Less M, Perl-Treves D, Primack H, et al. Continuous noninvasive glucose monitoring technology based on occlusion spectroscopy. *J Diabetes Sci Technol.* 2007;1(4):463–9.
37. Kohl M, Esseprens M, Cope M. The influence of glucose concentration upon the transport of light in tissue- simulating phantoms. *Phys Med Biol.* 1995;40:1267–87.
38. Kohl M, Cope M, Esseprens M, Böcker D. Influence of glucose concentration on light scattering in tissue- simulating phantoms. *Opt Lett.* 1994;19:2170–2.
39. Hill B. (ed.) *Accu-Chek advantage: electrochemistry for diabetes management, current separations.* 2014.
40. Hidalgo JI, Colmenar MJ, Risco-M JL, Maqueda E, Botella M, Rubio JA, et al. Clarke and Parkes error grid analysis of diabetic glucose models obtained with evolutionary computation, In proceedings of the 2014 conference companion on genetic and evolutionary computation companion (GECCO comp '14). New York: ACM; 2014. p. 1305–12.
41. Cox DJ, Clarke WL, Gonder-Frederick L, Pohl S, Hoover C, Snyder A, et al. Accuracy of perceiving blood glucose in IDDM. *Diabetes Care.* 1985;8(6):529–36.
42. Clarke WL, Gonder-Frederick LA, Carter W, Pohl SL. Evaluating clinical accuracy of systems for self-monitoring of blood glucose. *Diabetes Care.* 1987;10(5):622–8.
43. Kovatchev B, Gonder-Frederick LA, Cox DJ, Clarke WL. Evaluating the accuracy of continuous glucose monitoring sensors. *Diabetes Care.* 2004;27(8):1922–8.
44. Maran A, Crepaldi C, Tiengo A, Grassi G. Continuous subcutaneous glucose monitoring in diabetic patients. *Diabetes Care.* 2002;25:347–352.
45. Klonoff DC. Continuous glucose monitoring, roadmap for 21st century diabetes therapy. *Diabetes Care.* 2005;28:1231–9.
46. Guevara E, Gonzalez FJ. Joint optical-electrical technique for non-invasive glucose monitoring. *REVISTA MEXICANA DE FISICA.* 2010;56(5):430–4.
47. Facchinetti A, Sparacino G, Cobelli C. Reconstruction of glucose in plasma from interstitial fluid continuous glucose monitoring data: role of sensor calibration. *J Diabetes Sci Technol.* 2007;1(7):617–27.
48. Hariri A, Wang LY. Identification and low-complexity regime-switching-insulin control of type I diabetic patients. *J Biomed Sci Eng.* 2011;4:297–314.
49. Maxim-Vladimirovich S, Adriaan B, Nataliya-Lvovna S, Anton-Pavlovich T, Timur Alexandrovich J, Valeriy Anatol'evich K. Information technologies in modern industry, education & society. *World Applied Sciences Journal.* 2013;24:171–6.
50. Sharma JK. (ed.). *Business statistics,* Pearson Education India, 2012;463–464.
51. Vaddiraju S, Burgess DJ, Loannis T, Jain FC, Fotios P. Technologies for continuous glucose monitoring: current problems and future promises. *J Diabetes Sci Technol.* 2010;4(6):1540–62.
52. Oliver NS, Toumazou C, Cass AE, Johnston DG. Glucose sensors: a review of current and emerging technology. *Diabet Med.* 2009;26(3):197–210.

Error Grid Analysis of Reference and Predicted Blood Glucose Level Values as Obtained from the Normal and Prediabetic Human Volunteers

Md Koushik Chowdhury*, Anuj Srivastava, Neeraj Sharma, Shiru Sharma

School of Biomedical Engineering, Indian Institute of Technology, (Banaras Hindu University), Varanasi, India

Abstract Background: In this research paper, we represent a new noninvasive blood glucose level determining technology based on Amplitude Modulated Ultrasound and Infrared techniques. The successful advent of a noninvasive blood glucose determining technology will be helpful for patients with abnormal episodes of elevated Blood Glucose Levels. Noninvasive device will increase patient's compliances along with firm control over elevated Blood Glucose Levels (BGL). Moreover, it will reduce diabetes related medical emergency and burden from the shoulders of healthcare professionals. **Research Design:** A total of 10 adult human volunteers (02 Normal and 08 Prediabetic) had been engaged in this experimental pilot study. Main objective of these experiments are to analyze and compare the blood glucose levels as obtained from the established invasive (Accu-chek Active invasive blood glucose monitoring system from Roche Diagnostics) and indigenously developed noninvasive BGL determining technology (Amplitude Modulated Ultrasound and infrared Unit) respectively. The blood glucose levels after overnight fasting and 02 hour after meal had been observed in Normal and Prediabetic volunteers. Again following the next day, blood glucose level at fasting stage and 02 hour after 75gm/100ml glucose solution consumption had been monitored in those Normal and Prediabetic volunteers. Moreover, the invasive (reference) and noninvasive (predicted) blood glucose levels as obtained had been plotted over Clarke and Parkes Error Grids for evaluating indigenously developed technique performances. **Results:** The experimental findings reveal that Normal volunteers fasting blood glucose level exists more or less between (80-110) mg/dl. Similarly in separate pilot studies, their Blood Glucose Level varies more or less between (130-140) mg/dl after 02 hour of meal consumption and 75gm/100ml of glucose solution consumption respectively. But in case of Prediabetic volunteers, their fasting blood glucose level exists more or less above 110 mg/dl. Likewise in separate experimental studies, their Blood Glucose Level ranges more or less between (140-199) mg/dl after 02 hour of meal consumption and 02 hour after 75gm/100ml glucose solution consumption respectively. Moreover, the invasive (reference) and noninvasive (predicted) blood glucose levels of all the volunteers (normal and prediabetics) occupies medically significant and acceptable A and B zones in Clarke and Parkes Error Grids Analysis respectively. **Conclusions:** Experimental observations indicates the potential and prospective capability of our indigenously developed noninvasive Blood Glucose Level determining technique (Amplitude Modulated Ultrasound and Infrared unit) as revealed from the pilot studies over Normal and Prediabetic volunteers.

Keywords Clarke and Parkes Error Grid Analysis, Invasive, Noninvasive, Blood Glucose, Amplitude Modulated Ultrasound, Infrared Techniques

1. Introduction

Individual with elevated blood glucose level but not as much high as compared with diabetic patients are generally suffering from the IGT (Impaired Glucose Tolerance) or IFG (Impaired Fasting Glucose) related symptoms [1-3]. IGT refers to the medical condition in which blood glucose level elevates within the range between (140-199) mg/dl even two

hours after food consumption [1-3]. Similarly, the IFG refers to the medical situation where blood glucose level elevates above 110mg/dl even after overnight fasting time period [1-3]. The global populations resembling such typical symptoms are termed as prediabetics [1-3]. Consequently; the individuals with Prediabetic symptoms are severely prone to develop Type II Diabetes in near future [1-3]. Moreover, the IGT resembles Type II Diabetes symptoms adjunct with obesity, age progression, incapability of the human bodies to utilize insulin secreted from beta cells of the pancreas [1-3].

Complete change in lifestyle pattern, increased physical activity, controlled diet with low glycemic index food

* Corresponding author:

kchoudhary.rs.bme11@itbhu.ac.in (Md Koushik Chowdhury)

Published online at <http://journal.sapub.org/ajbe>

Copyright © 2015 Scientific & Academic Publishing. All Rights Reserved

consumption checks the progression of IGT towards Type II Diabetes Mellitus [1-3]. Globally 31.6 crores of people suffer from IGT related symptoms [1]. These numbers globally shares 6.9% of the present total adult population [1]. Moreover, large proportion of these population resides in lower as well as middle income territories. Worldwide 15.3 crores of the adult population suffer from these IGT symptoms within 50 year span of their life [1]. They also possess increased possibility to extend it towards Type II Diabetes Mellitus in later part of their life [1]. The global dominance of IGT resembles diabetes pervasiveness, with enormous proportion in African and European countries as compared to South-East Asian countries [1]. As per future estimations during the year 2035 A.D, 47.1 crores of peoples from the world population will suffer from IGT related symptoms or nearly 8.0% from the then total adult world population [1].

The crucial points of care for robust supervision of elevated blood glucose level include its 3 to 4 times regular monitoring on a daily basis [1-5]. Invasive glucometers rigorously perform such measurements each and every time with respective tissue puncturing procedures. Consequently the diabetic patients generally experiences mental agony for regular tissue puncturing and patient incomppliance occurs [3-5]. All this factors drives the urge for a nascent, novel noninvasive blood glucose determining technology with successful clinical applications [4, 5, 20-22]. In recent years, several optical techniques based noninvasive blood glucose level determining approaches had arrived with good potentiality and promising aspects [4-6, 20-22]. Such novel approaches mainly consists of Infrared Spectroscopy [7, 8, 20-22], Raman Spectroscopy [9, 20-22], Scattering Spectroscopy [10], Fluorescent Spectroscopy [11, 20-22], Polarimetry [12, 13, 20-22], Thermal Gradient Spectroscopy [14, 20-22], Photo-Acoustic Technology [15, 20-22], OCT (Optical Coherence Tomography) [16, 20-22], Occlusion Spectroscopy [17, 20-22], Photo-Thermal Technology [18], Ultrasound-Modulated Optical Techniques [19], etc.

The blood glucose exhibit weak signals and overlapped by numerous interferences from the surrounding optically active similar molecules [20-22]. To override such signal interferences we had applied Amplitude Modulated Ultrasound and Infrared Techniques altogether here. Moreover, this research paper focuses on the performance evaluation of indigenously developed noninvasive technique for determination of blood glucose levels in Normal and Prediabetic human volunteers.

Rest of Research Paper organizations are as follows: Section II describes the principle and working methodology. Section III illustrates the Instrumental block diagram, light wavelength and ultrasound band selection criteria. Section IV contains the experimental results and discussion portions. Section V provides the conclusive part of the research paper followed by acknowledgment and references.

2. Principle and Working Methodology

Noninvasive technique includes mainly amplitude modulated ultrasonic waves, infrared light beam and its respective IR (Infra Red) detector for determining blood glucose levels in Normal and Prediabetic Human Volunteers.

When standing ultrasonic waves propagates through the finger based blood tissue complex medium of human volunteers, it initiates the process of vibration throughout that respective medium. The molecules vibrate depending upon their respective mass, physical, chemical properties [23-25]. Moreover, the effect of radiation forces applied over the molecules had been derived from the gradient of molecular acoustic potential energy [23-32] and expressed as follows:

$$\mathbf{F}_r = - \left[\frac{\pi \rho_0^2 V_c \beta_w}{(2\lambda)} \right] \cdot \phi(\beta, \rho) \cdot \sin(4\pi z/\lambda) \quad (1)$$

The symbols like (\mathbf{F}_r), (\mathbf{V}_c), (\mathbf{z}), (\mathbf{P}_0), and (λ) stands for radiation force characteristics, volume of the respective molecules, space form the node of pressure, ultrasonic wave peak amplitude and wavelength of ultrasound respectively [23-32].

When compressibility aspects (β_w) of the suspending (blood tissue complex) segment present in human volunteers finger are considered, the mathematical expression had been represented as given below:

$$\phi(\beta, \rho) = \left[\frac{5\rho_c - 2\rho_w}{2\rho_c + \rho_w} - \left(\frac{\beta_c}{\beta_w} \right) \right] \quad (2)$$

The symbols like (β_c) stands for compressibility of the molecules and (ρ_c), (ρ_w) signifies molecular density of the suspending molecules and suspending segment respectively [23-32].

When infrared light beam propagates through these ultrasound (amplitude modulated ultrasonic waves) excited (blood tissue complex) optical medium, the glucose molecule vibration specific signatures are captured by the respective IR sensitive detectors. This light interaction phenomenon had been represented by Beer-Lambert Law [23-32] as follows:

$$\mathbf{A}(\mathbf{v}) = -\log \mathbf{I}(\mathbf{v})/\mathbf{I}_0(\mathbf{v}) \quad (3)$$

The symbols like (\mathbf{A}), (\mathbf{v}), (\mathbf{I}_0) and (\mathbf{I}) signifies Absorption patterns, wave number, light intensity from the surrounding medium and light intensity after transmission through the path length of measurement sample respectively [23-32].

3. MUS-IR Experimental Setup and Its Functional Part Depictions

Main functional parts of the MUS-IR Experimental setup had been illustrated as follows:

Synchronous square wave generator:

This functional part produces square wave based pulses to the IR LED (Infra Red Light Emitting Diode) light source.

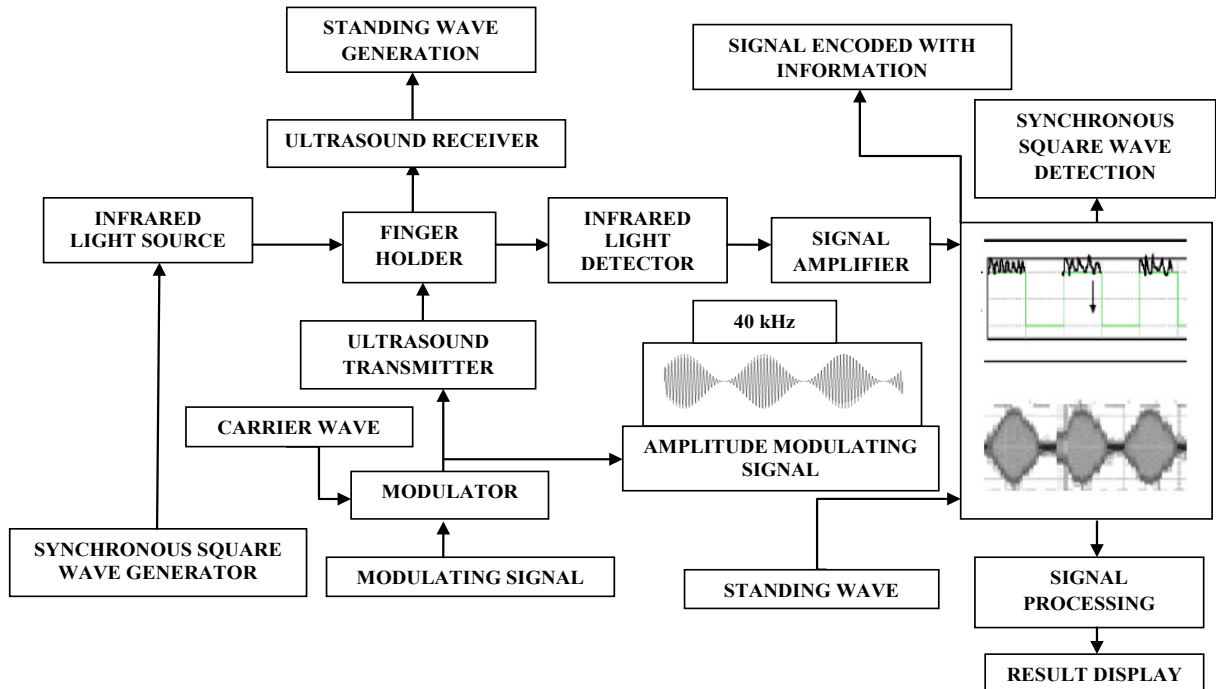


Figure 1. Block diagram of the MUS-IR (Modulated Ultra Sound-Infrared) Experimental Setup

Infrared light source:

IR LED of specific 940nm spectral wavelength had been selected and applied here. Actually 940nm occupies the position between “tissue optical window range” extending from 700nm to 1100nm [4, 33]. Within this zone the unwanted influence of other optically active molecules such as water, oxyhemoglobin, deoxyhemoglobin, etc. are reasonably negligible as depicted from Figure No.2, 4 respectively [4, 34-36]. Moreover, from Figure No.3 it can be revealed that glucose molecule exhibits absorption peaks near to 940nm wavelength [4, 34-36]

Modulating unit:

The modulating unit produces amplitude modulating standing wave pulses to UST (Ultra Sound Transmitter) unit. This functional component had been connected with two other primary parts such as carrier wave and modulating signal units.

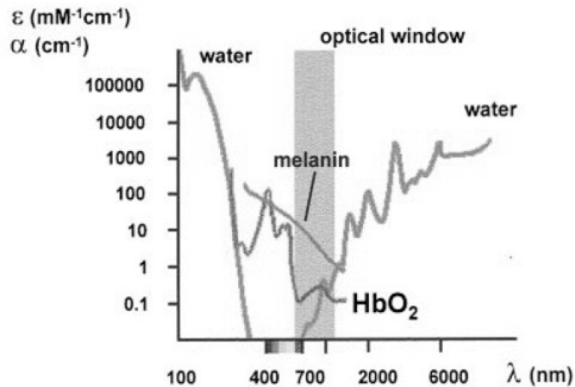


Figure 2. Absorption characteristics of chief intracellular components within the light spectral domain extending from 100nm to 6000nm [4, 33]

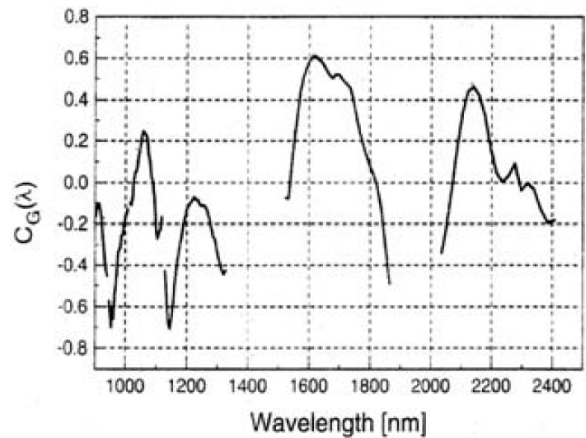


Figure 3. Absorption coefficient characteristics of Glucose within the light spectral domain extending from 900nm to 2400nm [4, 34-36]

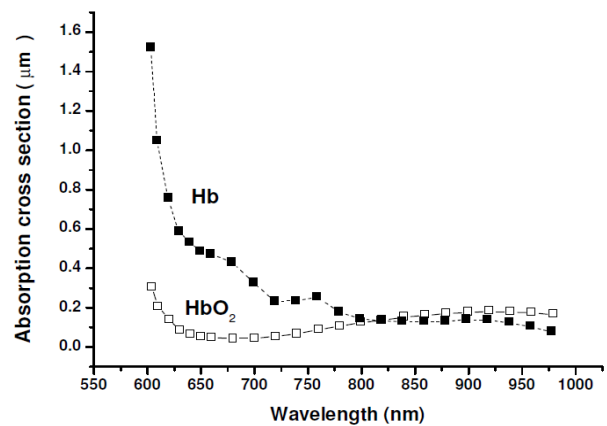


Figure 4. Absorption characteristics of Oxygenated Hemoglobin (HbO₂) and Deoxygenated Hemoglobin (Hb) within the light spectral domain extending from 550nm to 1000nm [4, 34-36]

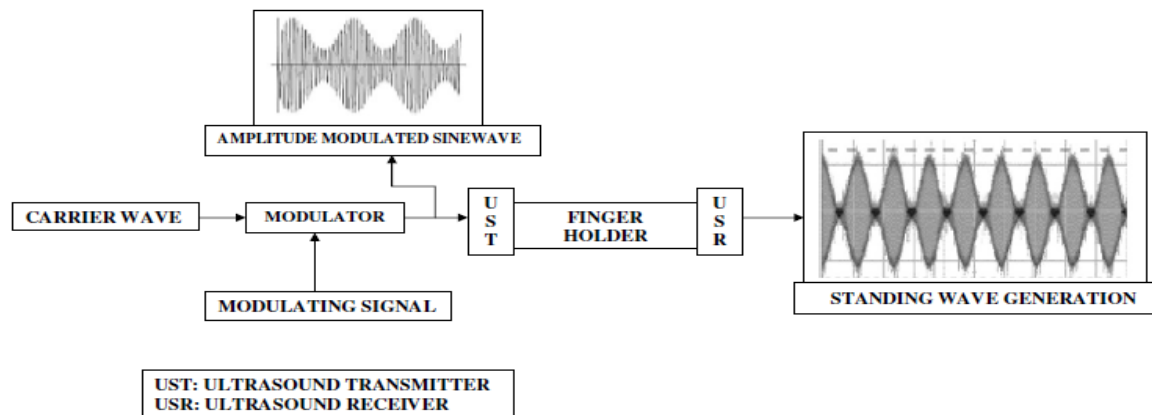


Figure 5. Shows the generation of amplitude modulated ultrasonic waves in MUS-IR Experimental unit

Ultra Sound Transmitter (UST):

Ultrasound Transmitter of 40 kHz central frequency had been selected and applied here. Actually the 40 kHz ultrasonic wavelength is medically safe for its use in human beings [24, 31, 32].

Moreover, amplitude modulated standing wave pulses as generated from the respective modulating unit serve as the signal input to UST unit. Consequently, the UST functional unit produces output signal in the form of ultrasonic amplitude modulated standing wave towards the finger holder unit. This phenomenon had been depicted here in the Figure No.5 as provided above.

Finger Holder Unit:

It upholds the human finger in precise geometrical position required for accurate IR light, ultrasonic wave transmission purposes. It helps in holding steady perpendicular orientation of IR light and ultrasonic unit with respect to finger positioning during signal acquisition periods. Moreover, it minimizes the unwanted errors such as motion related artifacts, wrong finger positioning, etc.

Ultra Sonic Receiver (USR):

Again, the Ultra Sonic Receiver of 40 kHz central frequency had been selected and applied here. Actually the 40 kHz ultrasonic wavelength is medically safe for its use in human beings [24, 31, 32]. USR unit checks the quality of ultrasonic waves generated from the UST unit. It is very important as it plays the key factor in blood glucose level determination purposes.

Infra Red (IR) detector:

It picks up the transmitted IR light signals and records the blood glucose specific vibrational patterns for its relevant concentration determinations.

Signal amplifier & processing unit:

This part performs the signal conditioning, amplifications and unwanted noise filtrations functions. Subsequently, the resultant signals were analyzed through the MATLAB toolbox to determine blood glucose concentration related embedded information. The peak to peak voltage amplitude

spectrum variations in FFT (Fast Fourier Transform) domain with respect to BGL (Blood Glucose Level) concentration were observed here. Actually, those typical voltage amplitude pattern variations serve as a functional indicator for respective change in the BGL levels.

Result Display:

This part of MUS-IR unit displays the noninvasive BGL (Blood Glucose Level) in mg/dl.

Clinical status of the Volunteers:

A group of 10 (seven males, three females, aged 35 ± 6.5 years, of height 173 ± 5.5 cm, weight 70 ± 11.5 kg) adult volunteers were selected. From which 02 volunteers are normal and healthy adults. Other 08 adult volunteers are with history of Prediabetic symptoms like IGT and IFT. Written consent had been obtained from all the volunteers. Institutional Ethical Committee approved the pilot study.

Clarke and Parkes Error Grid Analysis:

Clarke Error Grid analysis had been utilized to evaluate medical importance of the differentiations between blood glucose level predicting technique under examination and the established invasive blood glucose reference method. Clarke et al in the year 1986 A.D presented this novel analytical approach [37-42] and represents a Cartesian plot based diagrammatic approaches to characterize values of the reference (invasive) technology versus the predicted (predicted) technology [37-42]. As for illustration, if a human volunteer's Blood Glucose Levels is predicted to be 121 mg/dl for a particular moment where the reference BGL value is 113 mg/dl, this fact will be produced by the particular point as (113,121) in the XY Cartesian domains [37-42]. In this fashion, the diagonal line such as $Y=X$ symbolizes the ideal determinations, points under and over the diagonal line, designates over assessment and under assessment of the real BGL values. Interestingly, the Cartesian XY graph had been divided into several grid zones based on the degree of severity of miss judgments [37-42]. The Error Grid name also signifies these facts. Clarke et al divided the respective Cartesian graph into 05 different zones (A to E) [37-42] respectively, with the following interpretations as follows:

Zone A: signifies predicted blood glucose values which diverge as of the reference blood glucose values by 20% or less. It also include hypoglycemic ranges (<70mg/dl) of both the predicted and reference BGL values respectively [37-42]. These BGL values are medically accurate and suitable. For that, required medical supervision will be proper [37-42].

Zone B: signifies predicted BGL values which differ as of the reference BGL values by more than 20%. Within this zone we are nearer to medically erroneous BGL values but the medical supervision has an elevated likelihood of being accurate [37-42].

Zone C-E: the BGL values occupying those zones are extremely hazardous, as the determination or estimation is far away to be medically significant and the designated medical attention will differ from the accurate medical action required [37-42].

Parkes et al in the year 2000 A.D reentered the concept of respective zones and designed a new set of innovative error grids, based on the proficiency of big group of medical experts. These new Error Grids were designed differentiating for Type I and Type II diabetic subjects. Parkes Error Grids had been divided into 05 parts such as Zone A to Zone E respectively [43-45].

Zone A signifies medically correct determinations, with no consequence over medical supervision [43-45].

Zone B signifies changed medical action, minute or no consequences over medical treatment [43-45].

Zone C signifies changed medical action, probable to influence medical treatment [43-45].

Zone D signifies changed medical action, might comprise imperative medical jeopardy [43-45].

Zone E signifies changed medical action, might comprise unsafe effects [43-45].

Recently in the area of diabetes technology assessments, existence of the widely acceptable Consensus Error Grids (EGs) for checking errors between reference and predicted blood glucose level determinations is not available. For that reason, we had utilized both the available (Clarke and Parkes) Error Grids (EGs) for result analysis and evaluation purposes [37-45]

4. Experimental Results and Discussions

The experiments were conducted in two phases.

The Phase I includes determination of invasive (reference) and noninvasive (predicted) BGL values of both the Normal and Prediabetic volunteers after overnight fasting and after 02 hours of meal consumption.

The Phase II includes determination of invasive (reference) and noninvasive (predicted) BGL values of both the Normal and Prediabetic volunteers next day after overnight fasting and 02 hours after 75gm/100ml of glucose solution consumption.

For invasive blood glucose level determinations the Accu-chek Active blood glucose monitoring system of Roche Diagnostics GmbH had been utilized here. Similarly,

for noninvasive blood glucose level predictions we had utilized our indigenously designed and developed MUS-IR (Modulated Ultra Sound-Infra Red) unit.

Table No.1 and 2 shows the comparison of invasive (reference) and noninvasive (predicted) Blood Glucose Levels (BGL) as obtained from the Normal and Prediabetic subjects during Phase I and II experimental pilot studies respectively.

Both the invasive (reference) and noninvasive (predicted) results were plotted over Clarke and Parkes Error Grids for critical analysis purposes.

Figure No. 6(a) and 6 (b) depicts the Clarke and Parkes Error Grid Analysis based graphical plotting of the Invasive (reference) and Noninvasive (predicted) BGL values of the Normal and Prediabetic volunteers as acquired during the experimental pilot study respectively.

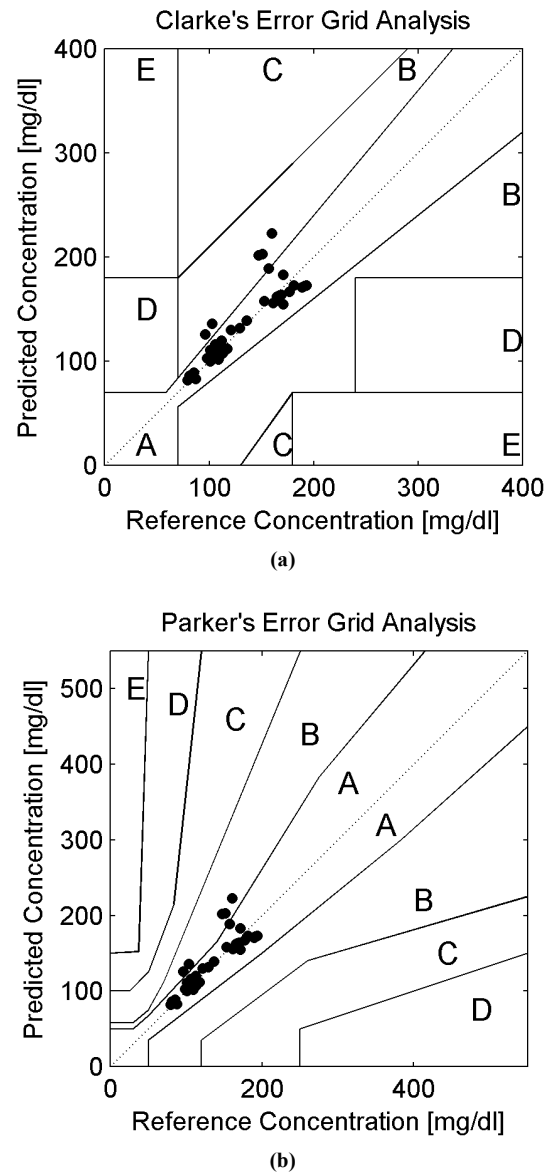


Figure 6. Represents Graphical depiction of Clarke and Parkes Error Grid Analysis of the invasive (reference) and noninvasive (predicted) BGL values as obtained from the Normal and Prediabetic subjects during the experimental pilot study respectively

Likewise, the Clarke Error Grid analysis based relevant BGL determining accurateness dependent proportional values as acquired from figure No.6 (a) are grouped as follows: A zone=85.00%, B zone=15.00%, C zone=00.00%, D zone=00.00% and E zone=00.00% respectively. Similarly, the Parkes Error Grid analysis based relevant BGL determining accurateness dependent proportional values as acquired from figure No.6 (b) are grouped as follows: A zone=85.00%, B zone=15.00%, C zone=00.00%, D zone=00.00% and E zone=00.00% respectively.

and noninvasive (predicted) BGL values as obtained during this experimental pilot study had been depicted in Figure No.7 (a) and 7 (b) respectively.

The Clarke Error Grid analysis based respective BGL determining accuracy dependent percentage values from figure No.7 (a) are categorized as follows: A zone=87.50%, B zone=12.50%, C zone=00.00%, D zone=00.00% and E zone=00.00% respectively. Correspondingly, the Parkes Error Grid analysis based respective BGL determining accuracy dependent percentage values from figure No.7 (b) are categorized as follows: A zone=87.50%, B zone=12.50%, C zone=00.00%, D zone=00.00% and E zone=00.00% respectively.

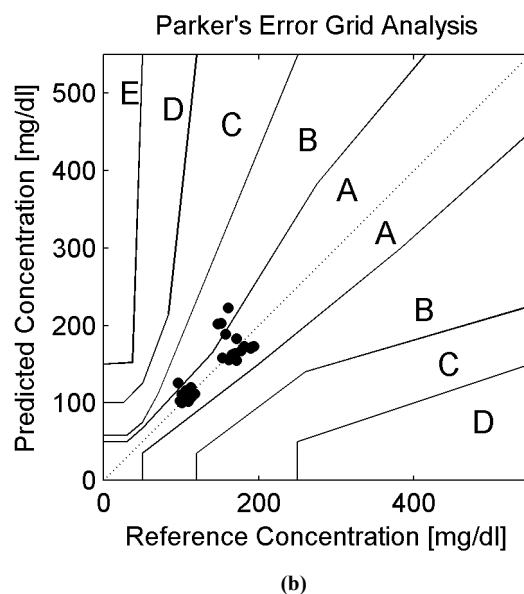
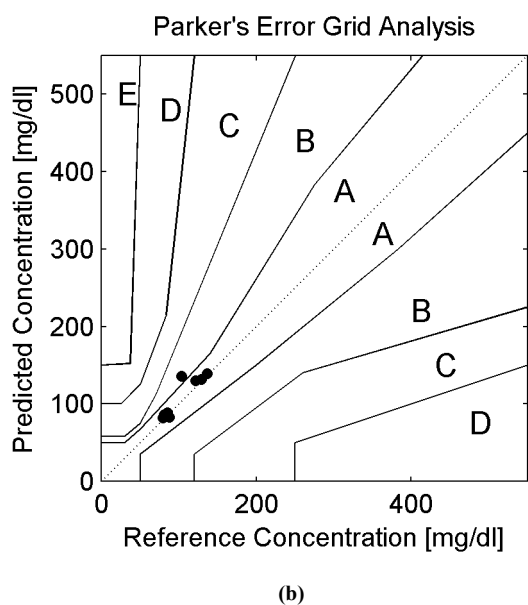
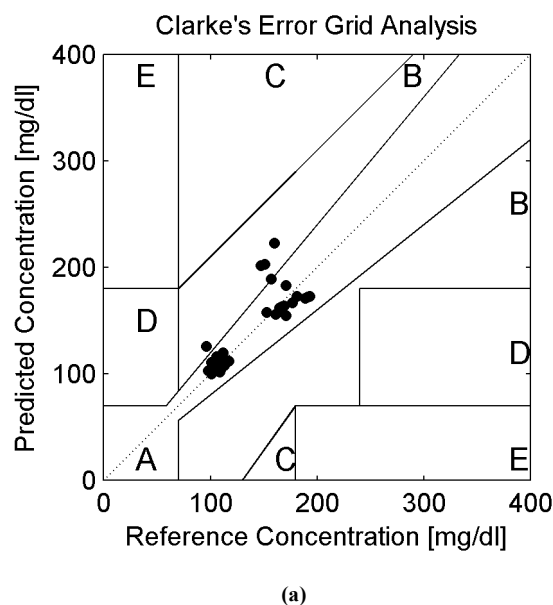
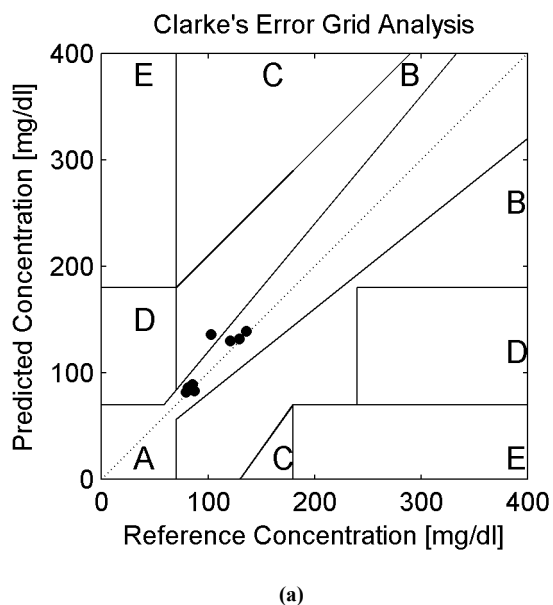


Figure 7. Represents Graphical depiction of Clarke and Parkes Error Grid Analysis of the invasive (reference) and noninvasive (predicted) BGL values as obtained from the Normal subjects during the experimental pilot study respectively

Clarke and Parkes Error Grid Analysis based graphical plotting for all the Normal volunteer's invasive (reference)

Figure 8. Represents Graphical depiction of Clarke and Parkes Error Grid Analysis of the invasive (reference) and noninvasive (predicted) BGL values as obtained from the Prediabetic subjects during the experimental pilot study respectively

Graphical plots in Figure No.8 (a) and 8 (b) respectively depict the Clarke and Parkes Error Grid Analysis for the Prediabetic volunteer's invasive (reference) and noninvasive (predicted) BGL values.

Moreover, the Clarke Error Grid Analysis based accuracy dependent percentage values of the BGL invasive (reference) and noninvasive (predicted) readings are classified as follows: A zone=84.3750%, B zone=15.6250%, C zone=00.00%, D zone=00.00% and E zone=00.00% respectively. Similarly, the Parkes Error Grid Analysis based accuracy dependent percentage values of the BGL readings are classified as follows: A zone=84.3750%, B zone=15.6250%, C zone=00.00%, D zone=00.00% and E zone=00.00% respectively.

Results obtained from analysis depicts that Prediabetic subject's blood glucose levels were elevated than normal physiological ranges but not as high compared to diabetic subjects during both the Fasting stage and 02 hr after meal or glucose solution consumption respectively. Similarly, for Normal subjects the blood glucose levels during Fasting stage and 02 hr after meal or glucose solution consumption are always within normal physiological range extending between (80-140) mg/dl.

Moreover, all the invasive and noninvasive BGL values

occupy the medically acceptable A and B zones respectively. This fact indicates dependable performance of our indigenously developed MUS-IR unit. All these results also correlate our previous blood glucose determination experimental values [24, 25, 31, 32]. The vital factor driving this technique comprises

- (i) Amplitude Modulated Ultrasonic wave utilizations for exciting specific molecules (glucose) present within the blood tissue complex.
- (ii) Specific and useful extraction of amplitude modulated ultrasound induced blood glucose concentration related information embedded signals from the transmitted infrared light.

The combined use of ultrasound and infrared light provides a new dimension for noninvasive detection of blood glucose levels. Few unwanted, erroneous signals had been obtained due to various types of factors like skin tissue related pigmentations, background light intensity, pulsatile flow of blood, machine related drifts, time dependent drifts, motion related artifacts, other physiological or pathological factors, etc. All these interfering sources modify the blood tissue complex induced bio signals and provide erroneous impact over blood glucose level determinations.

Table 1. Shows the comparison of invasive (reference) and noninvasive (predicted) Blood Glucose Levels (BGL) as obtained from the Normal subjects during Phase I and II experimental pilot studies respectively

NORMAL SUBJECTS	BLOOD GLUCOSE LEVEL (mg/dl)							
	Phase I				Phase II			
	BGL (mg/dl) After Overnight Fasting		BGL (mg/dl) 2hr After Meal Consumption		BGL (mg/dl) After Overnight Fasting		BGL (mg/dl) 2 hr after 75 gm/100ml Glucose Solution Consumption	
	Invasive method	Noninvasive method	Invasive method	Noninvasive method	Invasive method	Noninvasive method	Invasive method	Noninvasive method
SUBJECT1	81	86	103	136	79	82	121	130
SUBJECT2	85	89	136	139	87	83	129	132

Table 2. Shows the comparison of invasive (reference) and noninvasive (predicted) Blood Glucose Levels (BGL) as obtained from the Prediabetic subjects during Phase I and II experimental pilot studies respectively

PREDIABETIC SUBJECTS	BLOOD GLUCOSE LEVEL (mg/dl)							
	Phase I				Phase II			
	BGL (mg/dl) After Overnight Fasting		BGL (mg/dl) 2hr After Meal Consumption		BGL (mg/dl) After Overnight Fasting		BGL (mg/dl) 2 hr after 75 gm/100ml Glucose Solution Consumption	
	Invasive method	Noninvasive method	Invasive method	Noninvasive method	Invasive method	Noninvasive method	Invasive method	Noninvasive method
SUBJECT3	101	100	177	167	106	116	151	203
SUBJECT4	107	109	169	164	109	102	171	183
SUBJECT5	115	112	165	162	107	104	189	171
SUBJECT6	107	104	161	156	101	111	167	163
SUBJECT7	113	108	153	158	110	105	193	173
SUBJECT8	110	114	181	173	96	126	160	223
SUBJECT9	98	103	191	172	112	120	147	202
SUBJECT10	105	110	171	155	117	112	157	189

5. Conclusions

The hybridized potential aspect of utilizing amplitude modulated ultrasound and Infra Red technique for determining noninvasive blood glucose levels had been reported in this research paper. For cross validations of acquired noninvasive BGL values, the invasive glucometer of Roche diagnostics had been applied here. Furthermore, the 940nm LED and 40 kHz-generating central frequency based Ultrasound Transmitter forms the main instrumental base for this noninvasive technology. For validating the performance of noninvasive blood glucose detecting technology the Error Grid Analytical approaches had also been applied here. Error Grid Analysis shows that all the invasive (reference) and noninvasive (predicted) BGL values occupy within the medically significant A and B zones.

At present all new noninvasive BGL determining techniques requires invasive glucose sensors for calibration purposes. Hope our nascent noninvasive BGL determining technology will be successful in near future with all the aspects.

ACKNOWLEDGMENTS

All authors of the manuscript wish to appreciate the Coordinator and other Faculty members of School of Biomedical Engineering, IIT-(BHU), Varanasi for their support during the experimental works and manuscript writing.

REFERENCES

- [1] International Diabetes Federation, "IDF Diabetes Atlas," 6th Edn. Brussels, Belgium: International Diabetes Federation (2013). <http://www.idf.org/diabetesatlas>.
- [2] P. J. Watkins, Ed., "ABC of Diabetes", 5th ed., London: BMJ Books, 2003.
- [3] <http://diabetes.webmd.com/>.
- [4] Tuchin V.V, Ed., "Handbook of Optical Sensing of Glucose in Biological Fluids and Tissues". 1st Edn., CRC Press, Taylor & Francis Group, London, 2009.
- [5] A. Tura, A. Maran and G. Pacini, "Non-invasive glucose monitoring: Assessment of technologies and devices according to quantitative criteria", *Diabetes Research and Clinical Practice*, vol. 77, pp.16-40, 2007.
- [6] "Special issue on non-invasive glucose monitoring with optical technique", *IEEE Leos Newsletter*, April, 1998.
- [7] J. Tenhunen, H. Kopola, and R. Myllyla, "Non-invasive glucose measurement based on selective near infrared absorption: requirements on instrumentation and special range," *Measurement*, vol.24, pp.173–177, 1998.
- [8] J.S. Maier, S.A. Walker, S. Fantini, M.A. Franceschini, and E. Gratton, "Possible correlation between blood glucose concentration and the reduced scattering coefficient of tissues in the near infrared," *Opt. Lett.*, vol. 19, pp.2062–2064, 1994.
- [9] A.M.K. Enejder, T.G. Sceecina, J. Oh, M. Hunter, W.-C. Shih, S. Sasic, G.L. Horowitz, and M. S. Feld, "Raman spectroscopy for noninvasive glucose measurements," *J. Biomed. Opt.*, vol. 10, 2005, 031114.
- [10] O.S. Abdalsalam, A.A. Awouda, "Noninvasive glucose monitoring using scattering spectroscopy", *American Journal of Biomedical Engineering* vol.4(3), pp.53-59, 2014.
- [11] J. Lakowicz and B. Maliwal, "Optical sensing of glucose using phase modulation fluorimetry," *Anal.Chim.Acta*, vol.271, pp.155–164, 1993.
- [12] S. Bockle, L. Rovati, and R.R. Ansari, "Polarimetric glucose sensing using the Brewster-reflection off-eye lens: theoretical analysis," *Proc. SPIE*, vol. 4624, pp.160–164, 2002.
- [13] C. Chou, C.Y. Han, W.C. Kuo, Y.C. Huang, C.M. Feng, and J.C. Shyu, "Noninvasive glucose monitoring in vivo with an optical heterodyne polarimeter," *Appl. Opt.*, Vol. 37, pp. 3553–3557, 1998.
- [14] S. Yeh, C. F. Hanna, S. Kantor, et al., "Differences in thermal optical response between intact diabetic and nondiabetic human skin," *Proc. SPIE*, vol.4958, pp. 213–224, 2003.
- [15] Z. Zhao, "Pulsed Photoacoustic Techniques and Glucose Determination in Human Blood and Tissue", Doctoral Thesis, University of Oulu, Finland, 2002.
- [16] K.V. Larin, M.S. Eledrisi, M. Motamedi, R.O. Esenaliev, "Noninvasive blood glucose monitoring with optical coherence tomography: a pilot study in human subjects," *Diabetes Care*, vol. 25, no. 12, pp. 2263–2267, 2002.
- [17] Orna Amir et al. "Continuous noninvasive glucose monitoring technology based on Occlusion spectroscopy," *Journal of Diabetes Science and Technology*, vol.1 (4), July, 2007.
- [18] H.S. Ashton, H.A. MacKenzie, P. Rae, Y.C. Shen, S. Spiers, et al., "Blood glucose measurements by photoacoustics," *CP463 Photoacoustic and Photothermal Phenomena: 10th International Conference*, pp. 570–572, 1999.
- [19] L. Zhu, J. Lin, B. Lin, H. Li., "Noninvasive blood glucose measurement by ultrasound-modulated optical technique", *Chinese Optical Letters*, vol.11(2), pp.021701-1 to 021701-5, 2013.
- [20] O. Khalil, "Noninvasive glucose measurement technologies: an update from 1999 to the dawn of the new Millenium," *Diabetes Technol. Ther.*, vol. 6, no. 5, pp. 660–697, 2004.
- [21] Md. K. Chowdhury, A. Srivastava, N. Sharma, S. Sharma, "Challenges & Countermeasures in Optical Noninvasive Blood Glucose Detection", *International Journal of Innovative Research in Science, Engineering and Technology (IJIRSET)*, vol.2, issue 1, Jan., pp.324-329, 2013.
- [22] A. Srivastava, Md. K. Chowdhury, S. Sharma, N. Sharma, "Blood Glucose Monitoring Using Non Invasive Optical Method: Design Limitations and Challenges", *International Journal of Advanced Research in Electrical, Electronics and Instrumentation Engineering (IJAREEIE)*, Vol. 2, issue 1, Jan., pp.615-620, 2013.

- [23] T. Haar, and S.J. Wyard, "Blood cell banding in ultrasonic standing wave fields: A physical analysis", *Ultrasound in Medicine and Biology*, vol. 4(2), pp.111-123, 1978.
- [24] Md. K. Chowdhury, A. Srivastava, S. Sharma, N. Sharma, "The potential application of amplitude modulated ultrasound with Infrared Technique for blood glucose level determination in non invasive manner". *Biomedical and Pharmacology Journal*, Vol.7, No.1, page no.195-206. (2014).
- [25] Md. K. Chowdhury, A. Srivastava, S. Sharma, N. Sharma, "Five days daily sessions of noninvasive blood glucose level predictions based on amplitude modulated ultrasound and infrared technique over a healthy and diabetic subject". *IOSR-Journal of Electrical and Electronics Engineering*, Vol.5.Ver. IV, pp-34-41, Sep-Oct.,2014.
- [26] S. Radel, M. Brandstetter, B. Lendl, "Observation of particles manipulated by ultrasound in close proximity to a cone-shaped infrared spectroscopy probe", *Ultrasonics*, vol. 50, pp.240–246, 2011.
- [27] W. T. Coakley, "Ultrasonic separations in analytical biotechnology", *Trends in Biotechnology*, pp. 506-511, 1997.
- [28] L.V. King, "On the acoustic radiation pressure on spheres", *Proceedings of the Royal Society of London* pp.212–240, A147, 1934.
- [29] K. Yosioka, Y. Kawasima, "Acoustic radiation pressure on a compressible sphere", *Acustica*, vol. 5, pp.167–173, 1955.
- [30] F. Petersson, A. Nilsson, C. Holm, H. Jonsson and T. Laurella, "Separation of lipids from blood utilizing ultrasonic standing waves in microfluidic channels", *The Analyst*, The Royal Society of Chemistry, vol.129, pp.938-943, 2004.
- [31] Md. K. Chowdhury, A. Srivastava, N. Sharma, S. Sharma, "The influence of blood glucose level upon the transport of light in diabetic and non-diabetic subjects". *International Journal of Biomedical and Advance Research*, vol.4 (5), pp.306-316, 2013.
- [32] A. Srivastava, Md. K. Chowdhury, S. Sharma, N. Sharma, "Optical Clearance Effect Determination of Glucose by near Infrared Technique: An Experimental Study using An Intralipid Based Tissue Phantom", *International Journal of Advances in Engineering & Technology (IJAET)*, Vol. 6 Issue 3, pp. 1097-1108, July, 2013.
- [33] K. Konig, "Multiphoton microscopy in life sciences", *Journal of Microscopy*, vol. 200-2, pp. 83-104, 2000.
- [34] J. Tenhunen, H. Kopola, and R. Myllyla, "Non-invasive glucose measurement based on selective near infrared absorption: requirements on instrumentation and special range," *Measurement*, vol. 24, pp. 173–177, 1998.
- [35] O.W. Assendelft, *Spectrophotometry of Hemoglobin Derivates*, Royal Vangorcum Ltd., Assen, 1970.
- [36] Y. Mendelson, "Pulse oximetry: theory and applications for noninvasive monitoring," *Clin. Chem.*, vol. 38, pp.1601–1607, 1992.
- [37] D. J. Cox, W. L. Clarke, L. G. Frederick, S. Pohl, C. Hoover, A. Snyder, L. Zimbelman, W. R. Carter, S. Bobbitt, and J. Pennebaker, "Accuracy of perceiving blood glucose in IDDM", *Diabetes Care*, vol. 8, no.6, pp. 529–536, 1985.
- [38] W. L. Clarke, L. A. G. Frederick, W. Carter, and S. L. Pohl, "Evaluating clinical accuracy of systems for self-monitoring of blood glucose", *Diabetes Care*, vol. 10, no. 5, pp. 622–628, 1987.
- [39] A. Maran et al. "Continuous Subcutaneous Glucose Monitoring in Diabetic Patients", *Diabetes Care*, Volume 25, Number 2, February, 2002.
- [40] B.P. Kovatchev et al. "Evaluating the Accuracy of Continuous Glucose Monitoring Sensors", *Diabetes Care*, Volume 27, Number 8, August, 2004.
- [41] E. Guevara and F. J. Gonzalez, "Prediction of Glucose Concentration by Impedance Phase Measurements", in *Medical Physics: Tenth Mexican Symposium on Medical Physics*, Mexico City (Mexico), vol. 1032, pp.259-261, 2008.
- [42] E. Guevara and F. J. Gonzalez, "Joint optical-electrical technique for noninvasive glucose monitoring", *Revista Mexicana De Fisica*, vol. 56, no. 5, pp. 430-434, Sep., 2010.
- [43] Parkes JL, Slatin SL, Pardo S, Ginsberg BH, "A new consensus error grid to evaluate the clinical significance of inaccuracies in the measurement of blood glucose", *Diabetes Care*, vol. 23(8), pp.1143–1148, 2000.
- [44] A. Pfitzner, D.C Klonoff, P Scott, J.L Parkes, "Technical Aspects of the Parkes Error Grid", *Journal of Diabetes Science and Technology*, vol.7(5), pp.1275-1281, 2013.
- [45] J. I Hidalgo, M. J Colmenar, J. L.Risco-M., E. Maqueda, M Botella, J.A Rubio, A.C. Infante, O Garnica, J Lanchares, 2014, "Clarke and Parkes error grid analysis of diabetic glucose models obtained with evolutionary computation", In *Proc., of the 2014 Conf. Companion on Genetic and Evolutionary Computation Companion (GECCO Comp '14)*. ACM, New York, NY, USA, 1305-1312.

The Error Grid Analysis of invasive and indigenously developed noninvasive technique based blood glucose readings obtained from the effect of various glucose concentration sample solutions over blood glucose levels on the human subjects

Chowdhury Koushik Md.* , Srivastava Anuj, Sharma Neeraj and Sharma Shiru

School of Biomedical Engineering, Indian Institute of Technology (Banaras Hindu University), Varanasi, Uttar Pradesh-221005, INDIA

*koushikvit.chowdhury@gmail.com

Abstract

Noninvasive blood glucose monitoring technology with significant clinical accurate measurement capability should have a beneficial impact over medical care system for diabetes and its related risk managements. Moreover blood or other body fluid less technology should increase patient compliances as well as robust control over fluctuating blood glucose levels. Herein, we represent the noninvasive technology and evaluate its efficiency for detecting the respective glucose concentration induced blood glucose levels on the human subjects. The purpose of this experiment was to observe the effect of various glucose concentration sample solutions like 25gm/100ml, 50gm/100ml and 75gm/100ml over blood glucose levels on the fasting 10 human subjects during the time duration of 1hour and 2hour after respective glucose solution consumptions. Moreover, the invasive and indigenous noninvasive technology based blood glucose level readings correlations were compared and evaluated through Clarke and Parkes Error Grid analytical approaches.

The experimental findings indicate that blood glucose levels increase with increase in concentration of glucose solutions in human subjects. At the same time, the blood glucose levels were regulated and controlled by the individuals' body glucose homeostasis response mechanisms. Similarly the Clarke and Parkes Error Grid analysis of the obtained invasive and noninvasive blood glucose readings showed that the measurement readings occupy the medically significant A and B zones respectively. Experimental study indicates the impact of glucose concentration over blood glucose levels and potential use of indigenously developed noninvasive technology based on amplitude modulated ultrasound with infrared technology for noninvasive blood glucose level determinations.

Keywords: Error Grid Analysis, Invasive, Noninvasive, Blood Glucose, Amplitude Modulated Ultrasound, I.R.

Introduction

Diabetes mellitus represents the medical condition in which excess amount of blood glucose circulates within the human body. It is often characterized as the hyperglycemic stage resulted due to impaired insulin release or action^{2,13,25,30}. Uncontrolled and abnormally elevated blood glucose concentrations for longer durations exert negative impact over the blood vessels, kidneys, eyes, nerves, heart etc. Severe pathological conditions like micro or macro Vascular diseases, Diabetic nephropathy, Diabetic retinopathy, Diabetic neuropathy, Diabetic foot ulcerations, Heart strokes etc.^{2,13,25,30} are the long term consequences of diabetes as the disease progresses^{13,30}. On the other side, too much or excessive insulin usage for maintaining normal blood glucose levels may sometime lead to life threatening situation known as excessive hypoglycemic attacks.

According to IDF (International Diabetes Federation), the 38.2 crores of recent world populations were diabetic. This figures will touch 59.2 crores mark within or before 25 years from now.¹⁵ Unfortunately 17.5 crores of today's world populations are unaware of diabetes prevalence in them and progressing towards diabetic related long term clinical consequences.¹⁵ Furthermore, 80% of the diabetic diseased population belongs to the lower and middle income territories of the world¹⁵. All these factors provide severe economical burden over the individuals suffering.

Rigid monitoring over the blood glucose levels in diabetic patients is vital for significant clinical management^{2,13,15,25,30}. The invasive glucometer provides self monitoring of blood glucose levels which employ tissue puncturing for collecting and analyzing blood samples¹¹⁻¹³. This procedure is painful and involves skin-tissue infection related clinical risks^{13,30}. To avoid such circumstances and for ease of self operations, several noninvasive blood glucose detecting technologies had been evolved in recent few decades.^{2,25} Such technologies comprise of Infrared Absorption, Near Infrared scattering, Raman spectroscopy, Fluorescent spectroscopy, Thermal gradient spectroscopy, Polarimetry, Polarization heterodyning techniques, Photonic crystal Technology, Photo acoustic Technology, Photo-thermal Technology, Optical Coherence Tomography (OCT) techniques and Ultrasound-modulated optical technique^{2,25,28}. The test sites for noninvasive blood glucose determinations comprise

mainly of the tip of fingers, finger web, forearms, ears, eyes etc.⁵. The experimental studies also include various skin layers and body fluids.⁵

The blood glucose molecule produces a very feeble signal which requires lots of designing complexity to acquire such weak signals.^{20,28,29} In order to overcome such difficulties, the amplitude modulated ultrasound with infrared techniques had been introduced here. This research article presents an indigenously developed noninvasive blood glucose detecting technology and evaluates its efficiency for detecting the respective glucose concentration induced blood glucose levels on the human subjects.

Materials and Methods

The principle combined effect of amplitude modulated ultrasound and infrared technique towards noninvasive blood glucose level detections: In this instrumental architecture principally we had utilized 940nm LED (Light Emitting Diode) as an Infrared (IR) light emitter and its respective IR detector. For ultrasonic wave generations we had selected a pair of 40 kHz Piezo-sensor based ultrasonic transmitter and receiver.

When two oppositely propagating ultrasonic waves combine with each other, the ultrasonic standing wave formation occurs³⁻⁵. These travelling waves can be generated from two separate transducers or from a transducer source and its respective reflector^{3-5,10,15,16,21,24,26,27,31}. The pressure amplitude of a standing wave has maximum and minimum values twofold above the distance of a unit wavelength. Within the propagating segment, discontinuities such as molecules achieve location specific acoustic potential energy due to its presence in the respective ultrasonic zone. Consequently, the progressions of the suspended molecules were observed towards the zone of least acoustic potential energy. Pressure nodes are usually nearer to these zones with respect to the molecules which are distanced from each other by path length of half a wavelength^{3-5,10,15,16,21,24,26,27,31}.

Similarly, when the molecular diameter is smaller than the wavelength of propagating ultrasound, the main force of radiation (F_r) acting on the molecule of volume (V_c), positioned by path of distance (z) from the pressure node is obtained from the gradient of the molecular acoustic potential energy^{3-5,10,15,16,21,24,26,27,31} and is expressed as:

$$F_r = - \left[\frac{\pi p_0^2 V_c \beta_w}{(2\lambda)} \right] \cdot \phi(\beta, \rho) \cdot \sin(4\pi z/\lambda) \quad (1)$$

Here, peak amplitude of the acoustic pressure has been symbolized as (P_0). The ultrasound wavelength in the suspending segment had been denoted as (λ). Compressibility of the suspending segment had been characterized as (β_w)^{3-5,10,15,16,21,24,26,27,31}. The mathematical expression of this phenomenon had been signified as:

$$\phi(\beta, \rho) = \left[\frac{5\rho_c - 2\rho_w}{2\rho_c + \rho_w} - \left(\frac{\beta_c}{\beta_w} \right) \right] \quad (2)$$

Similarly (β_c) stands for compressibility of the molecules. Notations (ρ_c) and (ρ_w) represent the respective densities of the molecules and the suspending segments.

Multiple factors were required to be measured when infrared spectral ranges were analyzed. Each and every sample delivers their unique IR signatures at a definite wave numbers^{5,24}. The well known Lambert-Beer law had been incorporated here to measure the specific absorption (A) properties at a definite light wave number (ν)^{5,24}. This observable fact had been expressed here as:

$$A(\nu) = -\log I(\nu)/I_0(\nu) \quad (3)$$

The background impact of light intensity had been denoted as (I_0) here. Similarly (I) represents the specific light intensity at the particular wave number (ν) of actual sample measurements.

Noninvasive blood glucose detecting Instrumental system

The IR LED of 940nm had been selected for noninvasive blood glucose level predictions. Actually figure nos.1 and 2 depict that the interference effect of other optically active substances like skin pigmentations induced melanin contents, water molecules, oxygenated hemoglobin and deoxy-hemoglobin etc. was reasonably less in that optical window range extending from 700nm to 1100nm^{5,17,28,29}. Furthermore, the absorption pattern of oxygenated hemoglobin and deoxy-hemoglobin as depicted from the fig. 3 is more or less similar in the wavelength band range between 900nm to 1000nm respectively^{1,19}. Consequently, the influence of oxygenation over the light absorption will be less in this zone^{1,5,17,19,28,29}. All this fact had directed us for selecting 940nm as the principle operating wavelength for noninvasive blood glucose level determinations^{5,17,28,29}.

The ultrasonic transmitter built in aluminum casings with 40 ± 1.0 kHz as centre frequency with driving voltage (RMS) of 30V had been utilized here. More over it is safe for its utilization over human beings. Additionally, easy commercial availability of both the items had encouraged us for their use in our experiments^{5,6}.

Instrumental system descriptions: Block diagram of the Modulated Ultra Sound-Infra Red (MUS-IR) unit for noninvasive blood glucose determinations had been represented in figure 4. Main functional parts of the instrumental system had been illustrated here as follows:

Square wave generator: This unit provides the square wave pulses in synchronous mode to the IR LED (Light Emitting Diode) light source.

IR LED: Infrared LED of 940nm (Thor Labs) had been utilized here as light source for the noninvasive blood glucose level determinations.

Modulator: This part had been connected with two other functional units like carrier wave and modulating signal unit respectively. It generates amplitude modulated signal as an input to the ultrasound transmitter unit.

UST (Ultra Sound Transmitter): The piezocrystal based ultrasound transmitter of 40 kHz as central frequency had been utilized here. Amplitude modulated input to the UST produces amplitude modulated ultrasonic waves. These unique waves were directed towards the finger holder section of the instrumental system.

Finger Holder: This part holds the human finger in correct fashion as required for the experimental purposes. The light and ultrasound sources were perpendicular in their respective geometrical orientations.

USR (Ultra Sound Receiver): This part provides cross checking of the unique standing wave pattern generated from the UST unit during calibration process of the instrument. The unique standing wave patterns of the amplitude modulated ultrasound play the important role for blood glucose level determinations in noninvasive manner. Consequently, the 40 kHz ultrasonic receiver had been incorporated here.

IR Detector: The detector incorporated here is very responsive in the infrared spectral region. It senses the minute changes due to the variation in the blood glucose levels.

Signal Amplifier: This part of the instrument amplifies the acquired bio-signal. At the same time it removes the unwanted noises from the acquired signal for obtaining good SNR (Signal to Noise ratio) values.

Signal Processing: This part performs the signal processing and conditioning procedures for extracting blood glucose related information from the acquired bio-signals.

Display: This part displays the predicted noninvasive blood glucose level values in gm/dl.

Invasive blood glucose determination: Invasive measurements were performed by the well known and established invasive glucometer known as Accu-chek Active blood glucose monitoring unit of Roche Diagnostics^{11,12}.

Human subject's medical profiles: Total of 10 human subjects was selected for this experiment. Eight of them were males and two are females aged between 22 to 29 years. Their height and weight vary in the range between

157cm to 165cm and 65kg to 79kg respectively. Objectives of the experimental protocols were briefed before the subjects; they all understood the procedures and their written consents were obtained. The Institutional Ethical Committee had approved the pilot study.

Experimental Protocol

Determine the effects of 25gm/100ml, 50gm/100ml, 75gm/100ml of glucose solution over fasting human individuals throughout the time period of 1hr and 2hr after its consumptions. Additionally, evaluate the working efficiency of the indigenously developed noninvasive technique based blood glucose level readings with respect to the standard invasive glucometer.

The experiments were conducted in the morning and the subjects were instructed to fast (water permitted) for 10 to 12 hours before the tests.

Step A: The noninvasive and invasive fasting blood glucose level of the human subjects was acquired at 0 min.

Step B: A glucose solution of 25gm/100ml (Approx.) of water was provided for drinking to the human subjects in a given time span of 5 minutes after step A.

Step C: This phase involves acquirement of noninvasive and invasive blood glucose level readings from all the 10 subjects after 1 hour and 2 hour of glucose solution consumptions respectively. Same steps were followed for 50gm/100ml and 75gm/100ml of glucose solution over 10 human subjects for next 2 days respectively.

For noninvasive determinations, all the obtained bio-signals were consecutively processed through the toolbox of MATLAB for obtaining the blood glucose level information. The peak to peak amplitude values in the FFT (Fast Fourier Domain) domain change with respect to the change in the blood glucose levels. This peak value serves as the functional indicator for the noninvasive blood glucose level determinations in this experimental procedure. Similarly, for invasive determinations Accu-chek active^{11,12} based blood glucose level readings were obtained and recorded accordingly.

Error Grid Analysis: The Clarke Error Grid Analysis had been utilized here to critically assess the medical importance of differences between the noninvasive blood glucose measurement technique under examination and invasive blood glucose monitoring glucometer as the reference measurements. Clarke et al.⁷ in the year 1986 had presented this methodology where the Cartesian diagram had been utilized to compute the predicted (noninvasive) blood glucose values against the invasive (real) blood glucose values^{6-9,18}. For instance, when the noninvasive (predicted) blood glucose value is 123mg/dl and the actual (invasive) blood glucose value obtained is 88 mg/dl, it will be expressed through the point as (88,123) in the Cartesian

XY coordinates. In this fashion the diagonal line where $Y=X$, expresses the ideal measurements¹⁴. The data points below and above the diagonal line represent the overestimation and underestimation of the real blood glucose values respectively.

Furthermore, the XY graph had been subdivided into several Grid zones which had been based on the degree of the miss calculations¹⁴. Clarke et al.⁷ had divided 5 zones in the respective XY-Cartesian graph with the following interpretations:

Zone A: It characterizes the blood glucose values that diverge away from the actual reference values by means of 20% or less and also the blood glucose values in the hypoglycemic ranges (less than 70mg/dl). These type of output values are medically correct and medical attention will be proper^{6-9,14}.

Zone B: It characterizes the blood glucose values that diverge from the actual reference values by means of more than 20%. This domain represents the starting of errors but medical treatment had a high possibility of being accurate. The data points under the Zone B are also medically significant and tolerable^{6-9,14}.

Zone C-E: The blood glucose values in those zones had been characterized as potentially dangerous and unacceptable. The predicted values were distance away from the real values and the medical treatment will be erroneous. High probabilities of medically significant errors occur due to those erroneous values in those respective zones^{6-9,14}.

Parkes et al.²² revisited the concept of the respective zones with a new dimension regarding error grids by utilizing the knowledge of a large group of expert medical physicians^{14,22,23}. Parkes Error Grid analysis differs for Type I diabetic subjects and Type II diabetic subjects respectively. The procedures of surveying 100 medical physicians of diabetes expertise were conducted to consign any errors starting from zone A to E as provided by the Clarke Error Grid. The Parkes Error Grid had been divided into 5 different zones^{14,22,23} such as:

Zone A represents medically correct blood glucose value determinations with no effect over the medical treatment.

Zone B represents misrepresented medical action, slight or less effect over the medical treatment^[14, 22, 23].

Zone C represents misrepresented medical action, prone to provide moderate effect over the medical treatment.

Zone D represents misrepresented medical action, might provide significant medical risk.

Zone E represents misrepresented medical action, might provide dangerous penalty.

At present, in the area of endocrinology common consensus for determining errors in the blood glucose value calculations do not exist¹⁴. For that we had utilized both the Error Grid based Analytical approaches for evaluating our respective results.

Results and Discussion

The effect of 25gm/100ml, 50gm/100ml, 75gm/100ml of glucose solution over the human subjects is seen within the time duration of 1hr and 2hr after the glucose solution consumptions respectively. The pattern of those values as seen from the table no. 1, 2 and 3 indicates that with increase in glucose concentration the blood glucose level increases but simultaneously the glucose levels were normalized by the body's physiological mechanisms.

At the same time, the noninvasive and invasive blood glucose levels were also measured to evaluate the working efficiency of the indigenously developed blood glucose detecting technology. The obtained values were critically analyzed through Clarke Error Grid and Parkes Error Grid analysis respectively. The graphical plotting of Clarke and Parkes Error Grid Analysis has been represented in figure 5 and 6 respectively. The values obtained from the Clarke Error Grid analysis were characterized as A zone=87.7778%, B zone=12.2222%, C zone=00.00%, D zone=00.00% and E zone=00.00% respectively.

Similarly, the values obtained from the Parkes Error Grid analysis were characterized as A zone=87.7778%, B zone=12.2222%, C zone=00.00%, D zone=00.00% and E zone=00.00% respectively.

The Error Grid Analysis shows that all the blood glucose values occupy the medical significant and acceptable zones like A and B respectively. All this directs towards the reliable efficiency of the indigenously developed amplitude modulated ultrasound and infrared technique based noninvasive blood glucose determining technology.

Similarly, the result of these experimental studies resembles our previous pilot study values^{4,5,25-27}. The important driving factor for this technology includes (a) appropriate utilization of the ultrasonic waves which is in amplitude modulating mode here; (b) Productive and standardized determination of blood glucose induced IR light signal patterns for noninvasive blood glucose level predictions.

The hybrid collaboration of amplitude modulating ultrasonic waves and the infrared methodology increases the blood glucose measuring perceptivity with good and medically acceptable correctness^{4,5,25-27}. A few erroneous signal based data had been acquired due to numerous typical factors like skin pigmentation issues, surrounding light, blood flow, machine drift, time drift, artifacts, other

biological factors etc.^{2,28,29} All these aspects alter the blood optical characteristics and induce effect over the actual blood glucose level measurement procedures.

Conclusion

The increase in effect of blood glucose level with increase in glucose concentration solution consumptions by the subjects and their respective physiological mechanism to control and lowering the individual’s blood glucose levels is observed. Moreover, the working capability of the indigenously developed noninvasive blood glucose determining technology had been evaluated through the

Clarke and Parkes Error Grid Analysis. The result obtained occupies the A and B zones in both the Error Grid (Clarke and Parkes) analysis which represents the good working efficiency of the indigenously developed noninvasive blood glucose detecting technology.

Acknowledgement

All the authors of the manuscript wish to thank the Coordinator and other faculty members of School of Biomedical Engineering, IIT-(BHU), Varanasi for their direct and indirect support throughout the experimental and the manuscript preparations procedures.

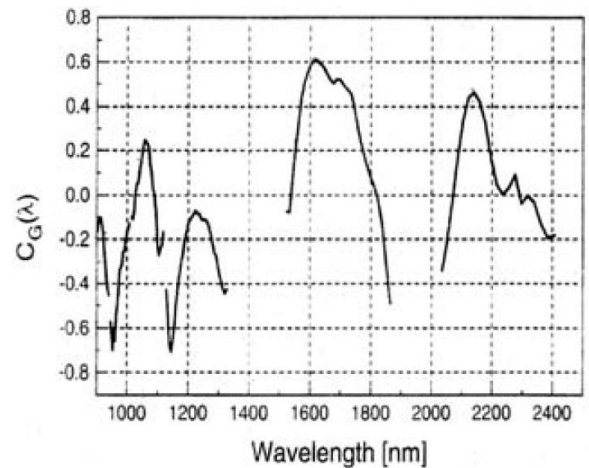
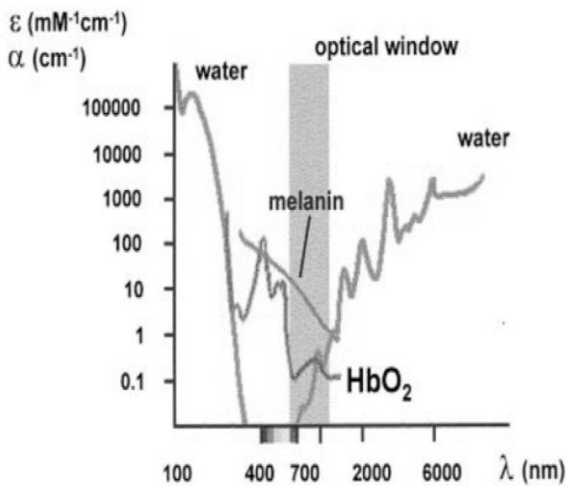


Figure 1: The range of major intracellular absorbers induced tissue optical window phenomenon in the wavelength spectrum starting from 100nm to 6000nm correspondingly¹⁷.

Figure 2: The absorption profile pattern of the glucose molecule in the wavelength spectrum starting from 1000nm to 2400nm correspondingly²⁹.

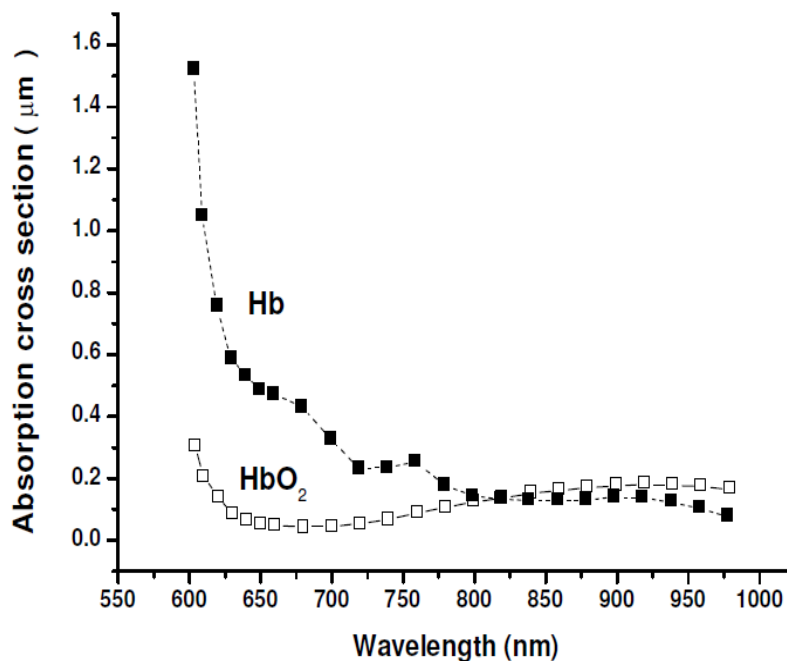


Figure 3: The absorption outline of the Hb (hemoglobin) and HbO₂ (oxygenated hemoglobin) in the wavelength spectrum starting from 550nm to 1000nm correspondingly^{1,19}.

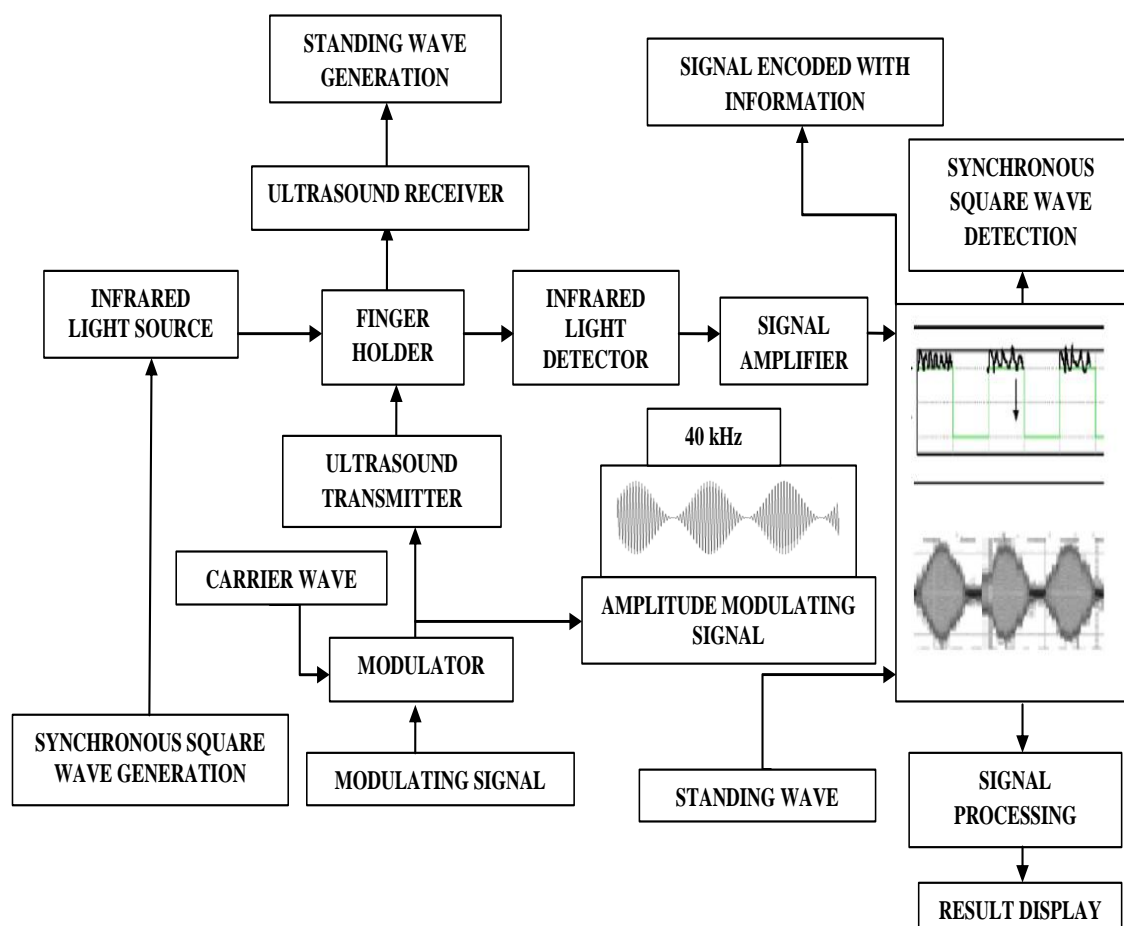


Figure 4: Outline of the noninvasive blood glucose determining instrumental system utilized during the experimental study.

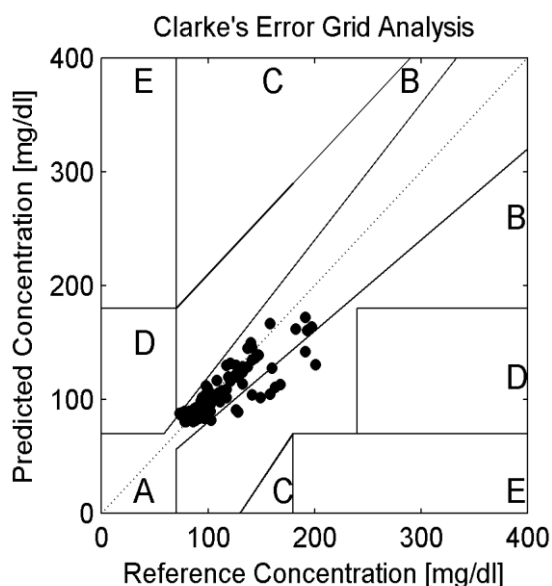


Figure 5: The Clarke's Error Grid based Analysis of the Blood Glucose Level values as acquired by the noninvasive (Predicted Concentration) and invasive (Reference Concentration) methods from all the subjects.

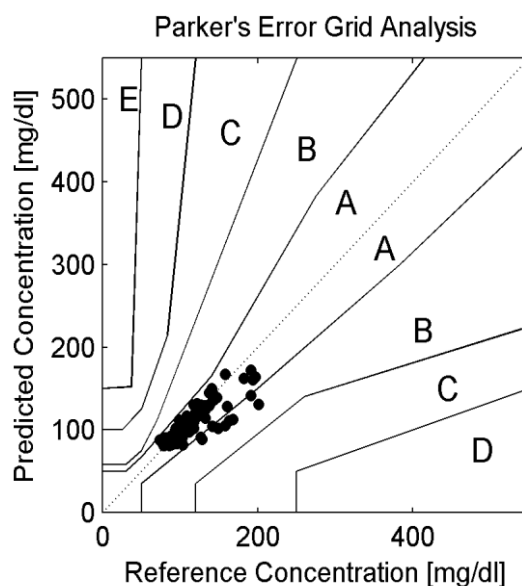


Figure 6: The Parkes Error Grid based Analysis of the Blood Glucose Level values as acquired by the noninvasive (Predicted Concentration) and invasive (Reference Concentration) methods from all the subjects.

Table 1

The respective invasive and noninvasive blood glucose levels (mg/dl) of all the subjects during fasting stage and after 1 hour, 2hour of 25gm/100ml of glucose solution consumption respectively

Subjects	Blood Glucose Level (mg/dl) during Fasting stage		Blood Glucose Level (mg/dl) after 1 hour of 25gm/100ml of glucose solution consumption		Blood Glucose Level (mg/dl) after 2 hour of 25gm/100ml of glucose solution consumption	
	Invasive blood glucose values as obtained by invasive glucometer (mg/dl)	Noninvasive blood glucose values as obtained by MUS-IR Unit (mg/dl)	Invasive blood glucose values as obtained by invasive glucometer (mg/dl)	Noninvasive blood glucose values as obtained by MUS-IR Unit (mg/dl)	Invasive blood glucose values as obtained by invasive glucometer (mg/dl)	Noninvasive blood glucose values as obtained by MUS-IR Unit (mg/dl)
Subject1	102	96	117	109	88	93
Subject2	92	86	127	120	94	102
Subject3	78	85	126	122	97	104
Subject4	81	86	132	124	112	105
Subject5	96	87	141	135	113	108
Subject6	92	86	144	137	100	108
Subject7	92	84	147	139	98	112
Subject8	94	87	137	145	108	117
Subject9	78	81	141	146	117	130
Subject10	79	82	140	150	121	132

Table 2

The respective invasive and noninvasive blood glucose levels (mg/dl) of all the subjects during fasting stage and after 1 hour, 2hour of 50gm/100ml of glucose solution consumption respectively.

Subjects	Blood Glucose Level (mg/dl) during Fasting stage		Blood Glucose Level (mg/dl) after 1 hour of 50gm/100ml of glucose solution consumption		Blood Glucose Level (mg/dl) after 2 hour of 50gm/100ml of glucose solution consumption	
	Invasive blood glucose values as obtained by invasive glucometer (mg/dl)	Noninvasive blood glucose values as obtained by MUS-IR Unit (mg/dl)	Invasive blood glucose values as obtained by invasive glucometer (mg/dl)	Noninvasive blood glucose values as obtained by MUS-IR Unit (mg/dl)	Invasive blood glucose values as obtained by invasive glucometer (mg/dl)	Noninvasive blood glucose values as obtained by MUS-IR Unit (mg/dl)
Subject1	77	86	110	106	98	100
Subject2	83	90	107	104	93	99
Subject3	94	91	111	98	103	82
Subject4	82	90	149	102	100	86
Subject5	77	85	117	102	102	90
Subject6	74	88	141	104	98	87
Subject7	77	89	158	105	88	86
Subject8	86	90	163	111	81	87
Subject9	79	81	168	113	78	86
Subject10	80	85	160	128	99	111

Table 3

The respective invasive and noninvasive blood glucose levels (mg/dl) of all the subjects during fasting stage and after 1 hour, 2hour of 75gm/100ml of glucose solution consumption respectively.

Subjects	Blood Glucose Level (mg/dl) during Fasting stage		Blood Glucose Level (mg/dl) after 1 hour of 75gm/100ml of glucose solution consumption		Blood Glucose Level (mg/dl) after 2 hour of 75gm/100ml of glucose solution consumption	
	Invasive blood glucose values as obtained by invasive glucometer (mg/dl)	Noninvasive blood glucose values as obtained by MUS-IR Unit (mg/dl)	Invasive blood glucose values as obtained by invasive glucometer (mg/dl)	Noninvasive blood glucose values as obtained by MUS-IR Unit (mg/dl)	Invasive blood glucose values as obtained by invasive glucometer (mg/dl)	Noninvasive blood glucose values as obtained by MUS-IR Unit (mg/dl)
Subject1	87	92	114	104	87	84
Subject2	91	94	129	122	88	85
Subject3	88	82	137	129	96	85
Subject4	96	84	201	131	128	89
Subject5	99	87	191	142	126	91
Subject6	78	90	182	162	132	114
Subject7	74	87	197	164	121	116
Subject8	73	88	158	167	119	120
Subject9	86	81	191	172	132	129
Subject10	81	87	193	161	126	130

References

- Assendelft O. W., Spectrophotometry of Hemoglobin Derivates, Royal Vangorcum Ltd., Assen (1970)
- Chowdhury Md. K., Srivastava A., Sharma N. and Sharma S., Challenges & Countermeasures in Optical Noninvasive Blood Glucose Detection, *International Journal of Innovative Research in Science, Engineering and Technology (IJIRSET)*, **2(1)**, 324-329 (2013)
- Coakley W. T., Ultrasonic separations in analytical biotechnology, *Trends in Biotechnology*, **15**, 506-511 (1997)
- Chowdhury Md. K., Srivastava A., Sharma N. and Sharma S., The influence of blood glucose level upon the transport of light in diabetic and non-diabetic subjects, *International Journal of Biomedical and Advance Research*, **4(5)**, 306-316 (2013)
- Chowdhury Md. K., Srivastava A., Sharma S. and Sharma N., The potential application of amplitude modulated ultrasound with Infrared Technique for blood glucose level determination in non invasive manner, *Biomedical and Pharmacology Journal*, **7(1)**, 195-206 (2014)
- Cox D. J., Clarke W. L., Gonder-Frederick L., Pohl S., Hoover C., Snyder A., Zimelman L., Carter W. R., Bobbitt S. and Pennebaker J., Accuracy of perceiving blood glucose in IDDM, *Diabetes Care*, **8(6)**, 529-536 (1985)
- Clarke W. L., Gonder-Frederick L., Carter A. W. and Pohl S. L., Evaluating clinical accuracy of systems for self-monitoring of blood glucose, *Diabetes Care*, **10(5)**, 622-628 (1987)
- Guevara E. and Gonzalez F. J., Prediction of Glucose Concentration by Impedance Phase Measurements, in MEDICAL PHYSICS: Tenth Mexican Symposium on Medical Physics, Mexico City (Mexico), **1032**, 259-261 (2008)
- Guevara E. and Gonzalez F. J., Joint optical-electrical technique for noninvasive glucose monitoring, *Revista Mexicana De Fisica*, **56(5)**, 430-434, (2010)
- Haar T. G. and Wyard S. J., Blood cell banding in ultrasonic standing wave fields: A physical analysis, *Ultrasound in Medicine and Biology*, **4(2)**, 111-123 (1978)
- Hill B., Accu-Chek Advantage: Electrochemistry for Diabetes Management, *Current Separations*, 45-48 (2014)
- <https://www.accu-chek.com/index.html> (2014)
- <http://diabetes.webmd.com/> (2014)
- Hidalgo J. I., Colmenar M. J., Risco M. J. L., Maqueda E., Botella M., Rubio J. A., Infante A. C., Garnica O. and Lanchares J., Clarke and Parkes error grid analysis of diabetic glucose models obtained with evolutionary computation, In Proceedings of the 2014 conference companion on Genetic and evolutionary computation companion (GECCO Comp '14), ACM, New York, NY, USA, 1305-1312 (2014)
- International Diabetes Federation, "IDF Diabetes Atlas," 6th ed., Brussels, Belgium: International diabetes Federation (2013), <http://www.idf.org/diabetesatlas> (2014)
- King L.V., On the acoustic radiation pressure on spheres, *Proceedings of the Royal Society of London*, **A147**, 212-240 (1934)
- Konig K., Multiphoton microscopy in life sciences, *Journal of Microscopy*, **200(2)**, 83-104 (2000)
- Kovatchev B. P. et al, Evaluating the Accuracy of Continuous Glucose-Monitoring Sensors, *Diabetes Care*, **27(8)**, 1922-1928 (2004)

19. Mendelson Y., Pulse oximetry: theory and applications for noninvasive monitoring, *Clin. Chem.*, **38**, 1601–1607 (1992)
20. Maran A. et al, Continuous Subcutaneous Glucose Monitoring in Diabetic Patients, *Diabetes Care*, **25**(2), February (2002)
21. Petersson F., Nilsson A., Holm C., Jonsson H. and Laurella T., Separation of lipids from blood utilizing ultrasonic standing waves in microfluidic channels, *The Analyst, The Royal Society of Chemistry*, **129**, 938-943 (2004)
22. Parkes J. L., Slatin S. L., Pardo S. and Ginsberg B. H., A new consensus error grid to evaluate the clinical significance of inaccuracies in the measurement of blood glucose, *Diabetes Care*, **23**(8), 1143–1148 (2000)
23. Pftzner A., Klonoff D. C., Scott P. and Parkes J. L., Technical Aspects of the Parkes Error Grid, *Journal of Diabetes Science and Technology*, **7**(5), 1275-1281 (2013)
24. Radel S., Brandstetter M. and Lendl B., Observation of particles manipulated by ultrasound in close proximity to a cone-shaped infrared spectroscopy probe, *Ultrasonics*, **50**, 240–246 (2010)
25. Srivastava A., Chowdhury Md. K., Sharma S. and Sharma N., Blood Glucose Monitoring Using Non Invasive Optical Method: Design Limitations and Challenges, *International Journal of Advanced Research in Electrical, Electronics and Instrumentation Engineering (IJAREEIE)*, **2**(1), 615-620 (2013)
26. Srivastava A., Chowdhury Md. K., Sharma S. and Sharma N., Optical Clearance Effect Determination of Glucose by near Infrared Technique: An Experimental Study using An Intralipid Based Tissue Phantom, *International Journal of Advances in Engineering & Technology (IJAET)*, **6**(3), 1097-1108 (2013)
27. Srivastava A., Chowdhury Md. K., Sharma S. and Sharma N., Measurement of Glucose Concentration using Amplitude Modulated Ultrasound with Infrared Technique in Intralipid Phantoms and Human Whole Blood mixed intralipid phantom of Healthy and Diabetic Subjects, *Bioscience Biotechnology Research Asia*, **11**(2), 593-602 (2014)
28. Special issue on non-invasive glucose monitoring with optical technique, IEEE Leos Newsletter, April (1998)
29. Tenhunen J., Kopola H. and Myllyla R., Non-invasive glucose measurement based on selective near infrared absorption: requirements on instrumentation and special range, *Measurement*, **24**, 173–177 (1998)
30. Watkins P. J., ABC of Diabetes, Fifth Edition, London, BMJ Books (2003)
31. Yosioka K. and Kawasima Y., Acoustic radiation pressure on a compressible sphere, *Acoustica*, **5**, 167–173 (1955).

(Received 29th September 2014, accepted 10th November 2014)

Estimation of fasting Blood glucose levels by invasive and indigenously developed noninvasive technology and its correlation with the glycated hemoglobin (HbA1c) biomarker in healthy and diabetic subjects

Chowdhury Koushik Md.^{*}, Srivastava Anuj, Sharma Neeraj and Sharma Shiru

School of Biomedical Engineering, Indian Institute of Technology (Banaras Hindu University), Varanasi, Uttar Pradesh-221005, INDIA

*koushikvit.chowdhury@gmail.com

Abstract

This research article represents the cross sectional study about the fasting glycemic index of normal and hyperglycemic subjects by invasive and indigenously developed noninvasive technology. Moreover, correlation between the fasting glycemic index and glycated hemoglobin (HbA1c) biomarker profile of both the normal and diabetic subjects has been analyzed and discussed. The fasting glycemic index measurements have been performed by the indigenous developed noninvasive method which utilizes both the amplitude modulated ultrasound and infrared techniques. The standing wave pattern of the ultrasound causes molecular vibration in the focused zone.

The infrared light based technology has been utilized to detect those glucose sensitive vibrational patterns to predict the glycemic index of the normal and diabetic subjects. Invasive fasting glycemic index and profile of glycated hemoglobin (HbA1c) biomarker were determined by the established invasive methods. The result emphasizes that both the invasive, noninvasive fasting glycemic index values change as the actual fasting glycemic index changes. Similarly, the glycated hemoglobin (HbA1c) biomarker profile of the diabetic subjects varies largely as compared to the normal subjects.

Keywords: Fasting glycemic levels, invasive, noninvasive, glycated hemoglobin (HbA1c), diabetic subjects.

Introduction

In the year 2013, according to the IDF (International Diabetes Federation) the diabetic population in India and worldwide is estimated to be around 6.51 and 38.2 crores respectively^{4,17,28}. This diabetic population prevalence in India and worldwide during the year 2035 may rise to 10.9 and 59.2 crores respectively^{4,17}. Moreover globally at present in 2013, the direct diabetes related treatment cost for different age groups had been more or less near to 581 billion international dollars¹⁷. Various projections indicate that it will be near to at least 678 billion international dollars status by the year 2035¹⁷. About half portion of the global diabetic population which had been estimated

around 17.5 crores peoples was undiagnosed for this metabolic disorder¹⁷. In the year 2013, global mortality rate indicates that nearly 5.1 and 1.1 million people died worldwide and in India respectively due to diabetic related complexity issues¹⁷. All this data reveal that every six seconds one person dies worldwide due to diabetic related disorders¹⁷.

As of 2013 data, our country India in the South-East Asian zone had been the major regional contributor for diabetes related mortality rate¹⁷. One Indian study reveals that mean glycated hemoglobin (HbA1c) biomarker level had been around 9.2% between 20,554 Type II Diabetic volunteers²¹. This marks towards the poor and weak glycemic management in our country^{21,25}. The consequences for this poor glycemic control in India count for 23.6% more macro and micro vascular neuropathy patients over the heart disease related patients^{21,25}.

The Glycated hemoglobin formation involves the amino-terminal valine moiety of hemoglobin β -chain combining with the glucose or hexose molecules. This bio-chemical process is slow, enzyme independent, irreversible substrate-concentration dependent and post translational in nature⁵. The glycated hemoglobin (HbA1c) biomarker efficacy for predictions, diagnosis, long term monitoring of Diabetes Mellitus profile had been an eminent methodology for rigorous investigations and discussion²². HbA1c level indicates the individuals plasma blood glucose homeostasis for past 60-90 days.^{5, 11, 18, 21, 22, 25, 29}

Moreover, impacts of the subject's current food diet regimen, psychological status cause negligible effect on the HbA1c levels^{5, 11, 18, 21, 22, 25, 29}. The count for HbA1c levels was the expedient and dependable diagnostic tools for accurate physiological glycemic levels projections^{11, 21, 22, 25, 29}. Higher values of HbA1c levels had been critically associated with diabetic related patho-physiological complications like cardiopathy, nephropathy, retinopathy, neuropathy etc.^{5, 11, 18, 21, 22, 25, 29} This metabolic disorder had taken the epidemic status worldwide triggering the research for the management of its long term complications and its related mortality, morbidity issues.

Material and Methods

Noninvasive technique based fasting blood glucose determination - Indigenously developed noninvasive MUS-IR unit operating principle for fasting blood

glucose level detections: In this technology we had utilized amplitude modulated ultrasonic waves and infrared light beam of desired wavelength. When ultrasonic sound beam amplitude modulating in nature propagates through the biological blood tissue complex matrix, it initiates vibrational properties into the medium^{5-8,14,19}. The force of radiations acting over the small diameter based molecules as compared with the ultrasonic wavelength were obtained from acoustic potential energy gradients of those molecules^{8,19,20,26,27,35} and represented as follows:

$$F_r = - \left[\frac{\pi p_0^2 V_c \beta_w}{2\lambda} \right] \cdot \phi(\beta, \rho) \cdot \sin(4\pi z/\lambda) \quad (1)$$

where F_r = character of the radiating force applied; V_c = molecular volumes of those molecules present in that blood tissue complex medium; z = distance; P_0 = peak amplitude of the acoustic pressure applied and λ = ultrasonic sound wavelength.

When the influences of the compressibility factors (β_w) of the suspending medium were accounted^{5-8,19,26,27,30,31,35}, the mathematical expressions were represented as follows:

$$\phi(\beta, \rho) = \left[\frac{5\rho_c - 2\rho_w}{2\rho_c + \rho_w} - \left(\frac{\beta_c}{\beta_w} \right) \right] \quad (2)$$

where β_c = compressibility of the molecules; ρ_c = molecular densities of the suspending molecules in that blood tissue complex medium and ρ_w = molecular densities of the suspending blood tissue complex medium.

When infrared light had been utilized to detect the glucose specific vibrational patterns for glucose concentration measurement, the standard Lambert-Beer law^{8, 26, 27, 30, 31, 35} principles were followed. The mathematical expression is as follows:

$$A(v) = -\log I(v)/I_0(v) \quad (3)$$

where A = Absorption profile; v = wave number of light wavelength; I_0 = surrounding medium light intensity and I = light intensity aftermath propagation through the blood tissue complex medium.

Noninvasive MUS-IR unit instrumental System Description: In this part, the indigenously developed noninvasive blood glucose instrumental system had been elaborated. The facts behind selection of light wavelength and ultrasonic transducer operating frequency were discussed. Subsequently, the instrumental setup description and procedures of the test performed had been explained.

Light wavelength and ultrasonic transducer operating frequency selection: The light emitting diode of 940nm had been chosen here. The impact of major intracellular absorbers like melanin, water, oxyhemoglobin, deoxy hemoglobin etc. were moderately low in the optical

window range between 700nm to 1100nm as depicted from the Figure 1 and 2 respectively^{1,20,23,32,33}.

Moreover, the absorption spectrum of the oxy hemoglobin and deoxy hemoglobin shows less dissimilarity in the range between 900nm to 1000nm as seen from the figure 3. The noise and interference from the other similar glucose like molecules were small in the range 700-1100nm of optical tissue window^{1,20,23,32,33}. As in Figure 2 glucose absorption peak near to 940nm wavelength drives the factor for 940nm light spectrum selection as the suitable source for blood glucose level predictions^{1,20,23,32,33}. Similarly, the safety aspect and wide availability of 40 kHz ultrasonic piezocrystal had also motivated us for its application in the experimental tests^{8,28,30,31}.

Block level depiction of the MUS-IR unit instrumental setup: Figure 4 depicts the block level description of the instrumental setup. The instrumental setup consists of amplitude modulating ultrasonic standing wave generator unit and the infra red light source-detector assembly. The square wave pulses supplied by the synchronous square wave generator focus typical square wave IR light pattern to the finger holder. Similarly amplitude modulating unit modulates the ultrasonic wave and directs those sound waves towards the finger holder. Both the light and ultrasonic units were perpendicular to each other. The infrared light focuses on the point of interaction of the amplitude modulating ultrasonic sound waves in the human finger based medium. The IR detector captures the resultant light signal.

After light signal acquisitions process, the signals undergo noise filtration and analysis through software toolbox of MATLAB. The peak to peak voltage amplitude spectrums in the FFT (Fast Fourier Transform) domain were observed here. The FFT Voltage amplitudes serve as a main function for blood glucose level determinations in noninvasive MUS-IR unit^{8,28,30,31}. The blood glucose embedded information was decoded and calculated to predict the respective glucose concentrations.

Invasive technique based fasting blood glucose determination: The invasive fasting blood glucose levels were determined by the Accu-Chek Active blood glucose monitoring device manufactured and marketed by Roche diagnostics GmbH. The invasive glucometer working accuracy had been based on the glucose dehydrogenase enzyme based typical electrochemical reactions and its measurements^{15,16}.

HbA1c determination methodology utilized: For in vitro quantitative glycosylated hemoglobin level determination in human blood we had utilized Ion Exchange Resin method^{2,3,24,34}. During column chromatography, the fast fraction glycosylated hemoglobins like HbA1a, HbA1b and HbA1c elute first in the columns due to lower isoelectric points. The bulk hemoglobin portions present there were

known as HbA₀ which is non-glycosylated in nature. The whole blood hemolysed sample preparations were introduced to the loosely binding cation-exchange resins beds^{2,3,24,34}. Labile fractions were expelled out during preparation of whole blood hemolysate samples and binding processes. During the mixing process, HbA₀ binds actively with the ion exchange beds leaving behind the GHb portion as a supernatant fraction.^{2,3,24,34}

Supernatant fractions rich in GHb portions were collected using filter separator after the mixing process. Absorbance of the Glycosylated Hemoglobin (GHb) fraction and the Total Hemoglobin (THb) fraction were measured at 415nm to determine the percentage of glycosylated hemoglobin^{2,3,24,34}. Subsequently, the absorbance ratio of the Glycosylated hemoglobin and the Total hemoglobin fraction of the Control and the Test were measured to estimate the percentage of Glycosylated hemoglobin in the samples. The range between (04.00%-20.0%) the Glycosylated hemoglobin procedure shows linearity. After that the standard conversion tables for GHbA1 in % to HbA1c in % values were followed to predict the HbA1c values^{2,3,24,34}.

Medical status of the Volunteers: A total of 20 volunteers (subjects), out of which 10 volunteers are normal healthy nondiabetic adults (seven males, three females, aged 26.6±2.0 years, of height 176±4.2cm, weight 74.6±12 kg), 10 volunteers with hyperglycemic conditions (six males, four females, aged 34±5.5 years, of height 172±4.5cm, weight 69±13.5 kg) were taken. Institutional Review Board permitted the pilot study. Informed written consent was obtained from all the volunteers before collecting the fasting samples.

Experimental protocol: Each and every volunteer was informed before 05 days of the experiments to continue their normal physical exercises and food habits. The volunteers were directed to have 12 hours overnight fasting before the examinations. The bio-specimen in form of blood samples were collected from the right arm artery for fasting invasive blood glucose level detection and Glycated hemoglobin level determination methodology. Simultaneously, the readings for noninvasive fasting blood glucose level determinations were obtained from the right hand index finger by the indigenously developed MUS-IR (Modulated Ultra Sound-Infra Red) unit.

Results and Discussion

Diabetes mellitus refers to a serious medical situation in which body blood glucose had been elevated and it prevails in uncontrolled manner. Tight glycemic level and diet control along with proper medications were extremely necessary for safe management of this metabolic disorder^{4,28}. Well managed blood glucose levels prevent patients from various life threatening diseases of heart, blood vessels, kidney, eyes, neurons etc.^{4,28} Technology advancement in the patient diagnostic field had emerged

the concept of noninvasive blood glucose detection methodology^{4,28}. The fasting (pre-prandial) result of our experimental clinical studies indicates that noninvasive method based MUS-IR unit had been working properly.

The noninvasive, invasive readings correlations were very good and acceptable as seen from table 1 and 2 and figure 8 and 9 for normal (1-10) and diabetic (11-20) subjects accordingly. The HbA1c values of the hyperglycemic subjects as seen in table 2 were higher as compared to the values in the table 1 of normal healthy subjects. Similarly figure 10 reveals the same fact of poor blood glucose level maintenance in hyperglycemic subjects (11-20) as compared with the normal subjects (1-10) HbA1c values over past 2 to 3 months. The Clarke error grid based analytical approach had been utilized here to evaluate medical significance of dissimilarity between the noninvasive blood glucose determination methodology based predictions under assessment and the established invasive blood glucose determinations as the reference one. This technique employs the Cartesian method based diagrammatic approaches. Under this technique, values predicted by the technique under evaluation were plotted on Y-axis and the values obtained from the reference method were plotted on X-axis.

The diagonal line linking the two technical aspects characterizes the zone of ideal concurrences. The Clarke error grid plot consists of five types of zones like zone A, zone B, zone C, zone D and zone E respectively. Zone A symbolizes for the predicted noninvasive blood glucose values that diverge from the reference invasive blood glucose values by margin of 20%. The values inside this domain are medically acceptable and contribute towards significant medical treatment. Zone B signifies the beginning of errors and the values again are in increment by 20%. Zone B values are also medically acceptable. The values within the zone from C and E are likely to be unsafe, and it can call for potentially serious, erroneous medical diagnosis and treatment^{9,10,12,13}. Here in this paper, figure 5 represents the Clarke error grid based percentage of total data for fasting blood glucose levels as obtained from the normal subjects (1-10). Values falling in the regions of A, B, C, D, E are 80.00%, 20.00%, 00%, 00% and 00% respectively.

Similarly, figure 6 corresponds to the percentage of total data for fasting blood glucose levels as obtained from the hyperglycemic or diabetic subjects (11-20). Values falling in the regions of A, B, C, D, E are 80.00%, 10%, 0%, 10% and 0% respectively. Again, the data points of normal (1-10) and hyperglycemic (11-20) subjects had been plotted altogether on the Clarke error grid platform as depicted from figure no. 7. The values obtained are as follows: A zone = 80%, B zone = 15%, C zone = 00%, D zone = 05% and E zone = 00% respectively. The result of this pilot study matches our earlier experimental values^{7,8,28,30,31}.

The vital factor for MUS-IR unit working includes (i) Suitable application of Amplitude Modulated Ultrasonic Standing waves (ii) Constructive and regular measurement of transmitted Infra red light signal based data for blood glucose level predictions. The collaboration of ultrasound and infrared techniques added up to the blood glucose measurement sensitiveness with high accuracy and precision^{7, 8, 28, 30, 31}. These entire phenomena direct us to use this hybrid technology for noninvasive blood glucose level detection purposes^{7, 8, 28, 30, 31}. A small number of erroneous signals were obtained due to various factors like pigmentation of skin, motion artifacts, unwanted light, pulsatile blood flow and other physiological factors etc. All these factors modify the blood optical properties to deviate the actual noninvasive readings.

Conclusion

We had represented the working principle of the MUS-IR unit for noninvasive blood glucose monitoring, which is based on modulated ultrasound and infrared technology. To evaluate the MUS-IR unit performances, the clinical pilot study were performed on healthy and diabetic volunteers. The noninvasive blood glucose readings showed a strong correlation with the invasive blood glucose readings and HbA1c values confirms the individual glucose tolerance loads.

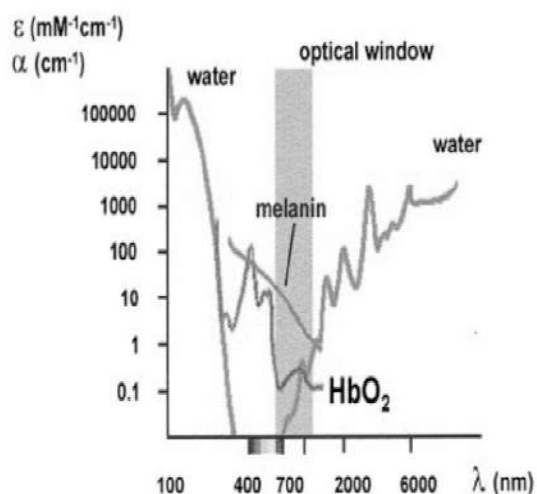


Figure 1: The tissue optical window phenomenon in the wavelength range from 100nm to 6000nm respectively²⁰.

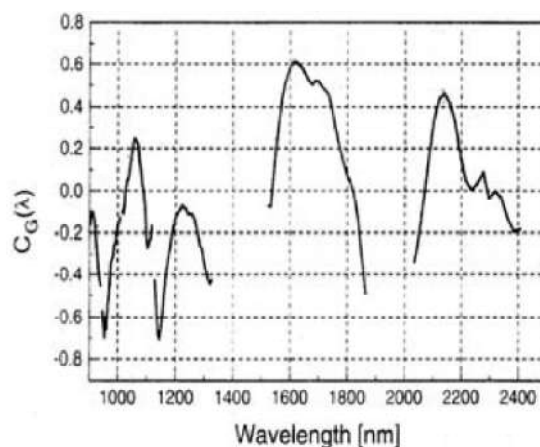


Figure 2: The glucose absorption pattern in the wavelength range from 900nm to 2400nm respectively³³.

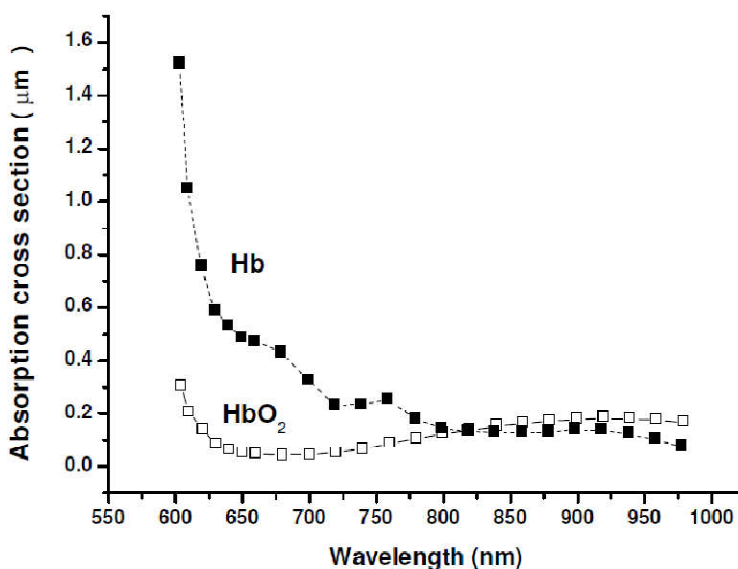


Figure 3: The absorption cross section pattern of the Hb (deoxy hemoglobin) and HbO₂ (oxygenated hemoglobin) in the wavelength ranges from 550nm to 1000nm respectively¹.

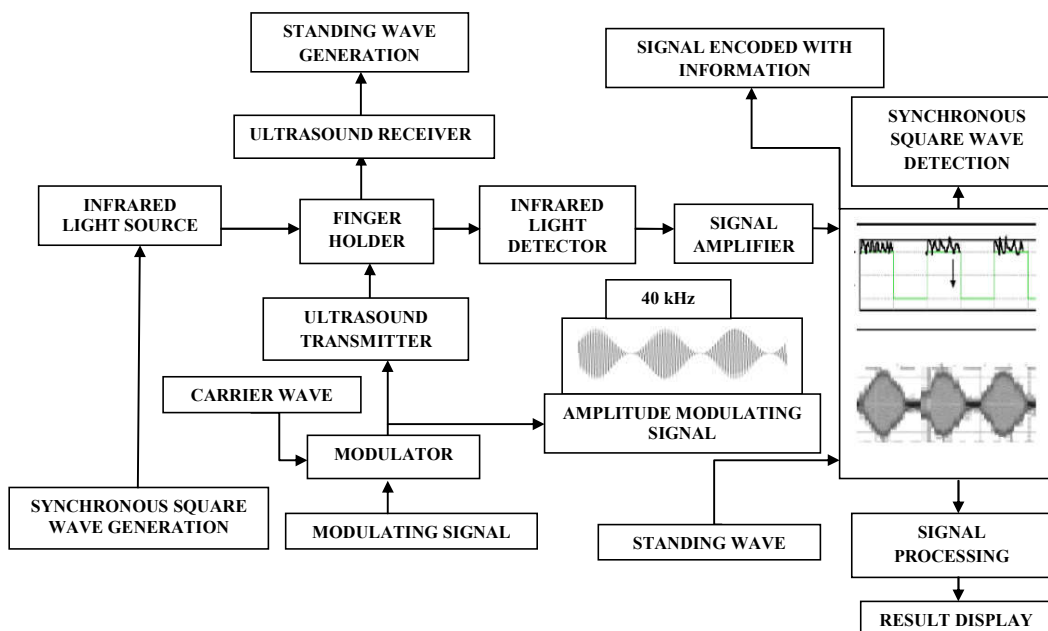


Figure 4: Sketch of the Amplitude Modulated Ultrasound and Infrared Technique based noninvasive blood glucose determining instrumental setup (MUS-IR Unit) utilized during the pilot study.

Table 1
Healthy volunteers invasive, noninvasive blood glucose values and GHb levels, HbA_{1c} values in percentage (%) respectively

S. N.	Healthy Volunteers	Invasive blood glucose values as obtained by invasive glucometer (mg/dl)	Noninvasive blood glucose values as obtained by MUS-IR Unit (mg/dl)	GHb levels in %	HbA _{1c} Values in %
1.	Subject 1	86.0	99.0	7.0	5.13
2.	Subject 2	76.0	90.0	6.7	4.88
3.	Subject 3	86.0	83.0	7.0	5.13
4.	Subject 4	71.0	88.0	6.5	4.71
5.	Subject 5	87.0	84.0	7.1	5.22
6.	Subject 6	95.0	91.0	7.4	5.47
7.	Subject 7	88.0	89.0	7.1	5.22
8.	Subject 8	90.0	87.0	7.2	5.30
9.	Subject 9	92.0	88.0	7.3	5.39
10.	Subject 10	105.0	81.0	7.7	5.72

Table 2
Diabetic volunteers invasive, noninvasive blood glucose values and GHb levels, HbA_{1c} values in percentage (%) respectively

S. N.	Diabetic Volunteers	Invasive blood glucose values as obtained by invasive glucometer (mg/dl)	Noninvasive blood glucose values as obtained by MUS-IR Unit (mg/dl)	GHb levels in %	HbA _{1c} Values in %
1.	Subject 11	141.0	139.0	9.0	6.81
2.	Subject 12	145.0	136.0	9.1	6.89
3.	Subject 13	181.0	167.0	10.4	7.98
4.	Subject 14	140.0	144.0	9.0	6.81
5.	Subject 15	148.0	146.0	9.2	6.98
6.	Subject 16	166.0	154.0	9.9	7.56
7.	Subject 17	159.0	161.0	9.6	7.31
8.	Subject 18	235.0	143.0	12.3	9.58
9.	Subject 19	165.0	161.0	9.8	7.48
10.	Subject 20	242.0	142.0	12.6	9.83

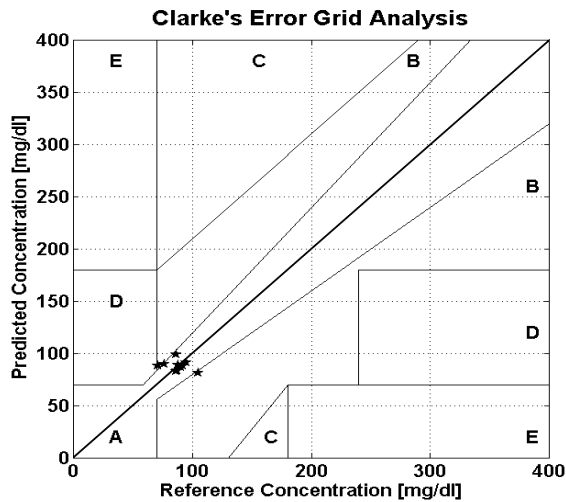


Fig. 5: Clarke's Error Grid Analysis of Invasive (Reference Concentration) and Noninvasive (Predicted Concentration) Blood Glucose levels as obtained from the Normal Healthy Subjects (1-10) respectively.

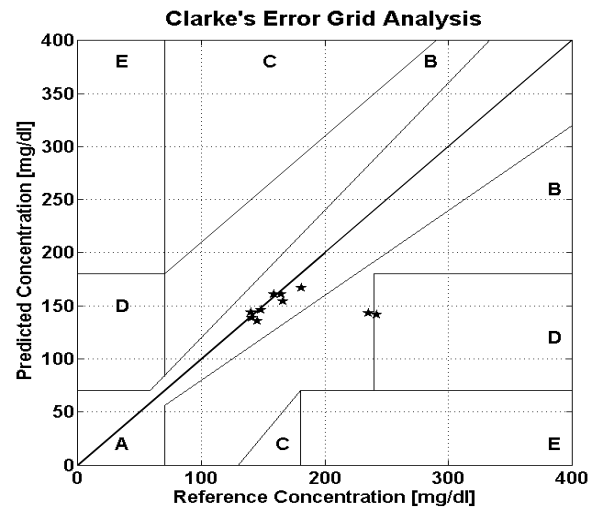


Fig. 6: Clarke's Error Grid Analysis of Invasive (Reference Concentration) and Noninvasive (Predicted Concentration) Blood Glucose levels as obtained from the Diabetic Subjects (11-20) respectively.

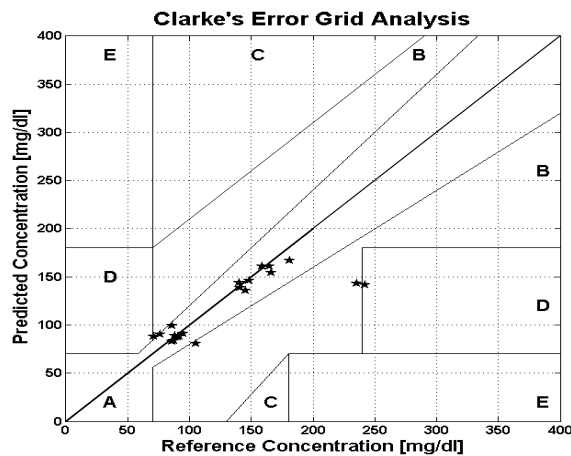


Fig. 7: Clarke's Error Grid Analysis of Invasive (Reference Concentration) and Noninvasive (Predicted Concentration) Blood Glucose levels as obtained from the Normal Healthy Subjects (1-10) and Diabetic Subjects (11-20) altogether respectively.

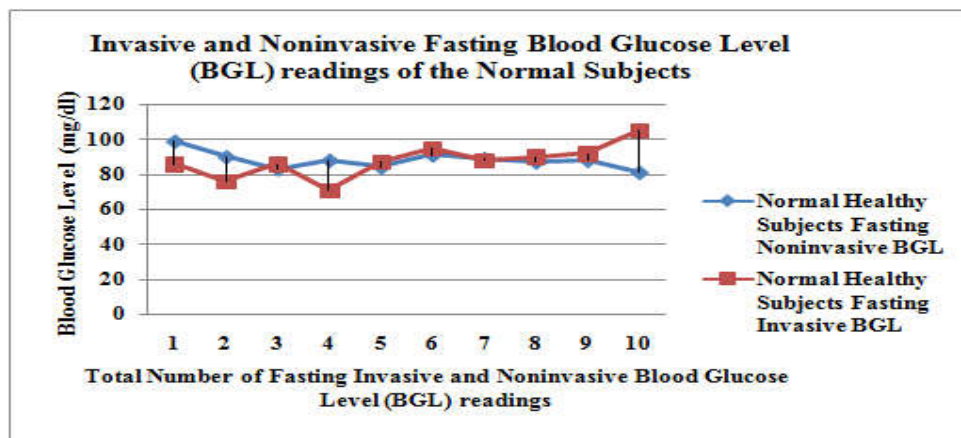


Fig. 8: Plotting of the Noninvasive and Invasive Fasting Blood Glucose Level (BGL) readings of the Normal Subjects (1-10) respectively.

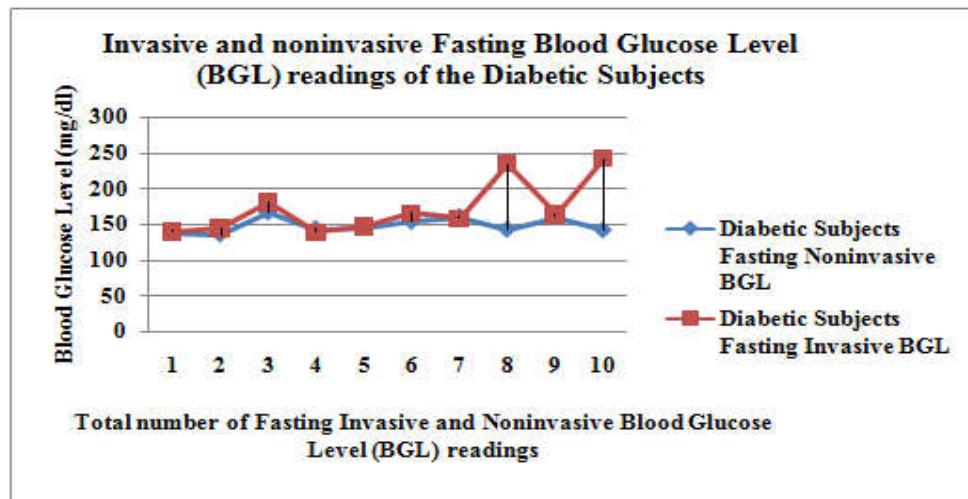


Fig. 9: Plotting of the Noninvasive and Invasive fasting Blood Glucose Level (BGL) readings of the Diabetic Subjects (11-20) respectively.

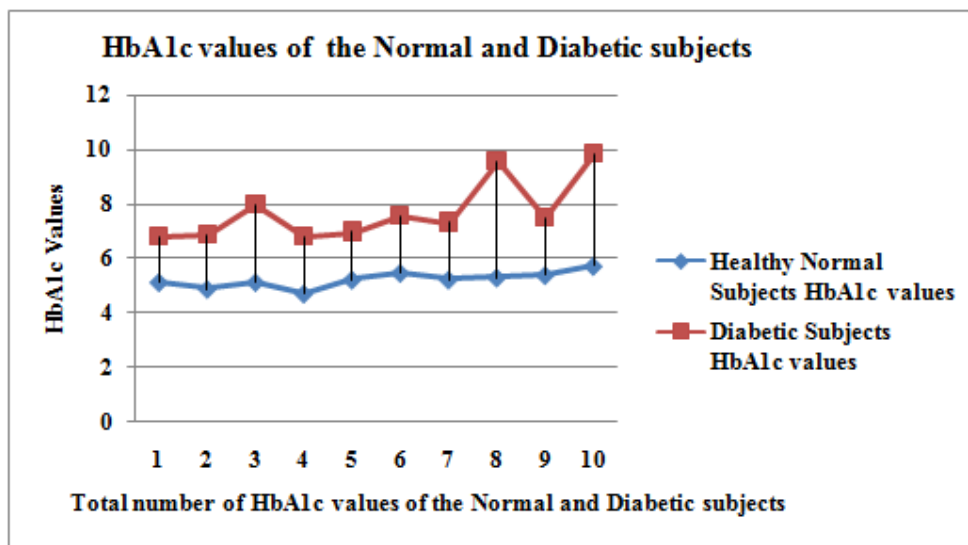


Fig. 10: Plotting of HbA1c values of the Normal (1-10) and Diabetic (11-20) Subjects respectively.

Acknowledgement

The authors were grateful to the Coordinator, Faculty members, Staff members of School of Biomedical Engineering, IIT-(BHU), Varanasi for their respective valuable supports during experimental pilot studies and manuscript writing.

References

1. Assendelft O. W., Spectrophotometry of Hemoglobin Derivates, Royal Vangorcum Ltd., Assen (1970)
2. Bunn H. F., *Diabetes*, **130**, 613 (1981)
3. Bates H. M., *Lab Manag.*, **16** (1978)
4. Chowdhury Md. K., Srivastava A., Sharma N. and Sharma S., Challenges & Countermeasures in Optical Noninvasive Blood Glucose Detection, *International Journal of Innovative Research*

in Science, Engineering and Technology (IJRSET), **2(1)**, 324-329 (2013)

5. Chandalia H. B. and Krishnaswamy P. R., Glycated Haemoglobin, *Current Science*, **83(12)**, 1522-1532 (2002)

6. Coakley W. T., Ultrasonic separations in analytical biotechnology, *Trends in Biotechnology*, **15**, 506-511 (1997)

7. Chowdhury Md. K., Srivastava A., Sharma N. and Sharma S., The influence of blood glucose level upon the transport of light in diabetic and non-diabetic subjects, *International Journal of Biomedical and Advance Research*, **4(5)**, 306-316 (2013)

8. Chowdhury Md. K., Srivastava A., Sharma S. and Sharma N., The potential application of amplitude modulated ultrasound with Infrared Technique for blood glucose level determination in non invasive manner, *Biomedical and Pharmacology Journal*, **7(1)**, 195-206 (2014)

9. Cox D. J., Clarke W. L., Gonder-Frederick L., Pohl S., Hoover C., Snyder A., Zimelman L., Carter W. R., Bobbitt S. and Pennebaker J., Accuracy of perceiving blood glucose in IDDM, *Diabetes Care*, **8(6)**, 529–536, (1985)
10. Clarke W. L., Gonder-Frederick L., Carter A. W. and Pohl S. L., Evaluating clinical accuracy of systems for self-monitoring of blood glucose, *Diabetes Care*, **10(5)**, 622–628, (1987)
11. Gomez-Perez F. J., Aguilar-Salinas C. A., Almeda-Valdes P., Cuevas-Ramos D., Lerman G. I. and Rull J. A., HbA1c for the diagnosis of diabetes mellitus in a developing country, A position article, *Arch Med Res*, **41(4)**, 302–308 (2010)
12. Guevara E. and Gonzalez F. J., Prediction of Glucose Concentration by Impedance Phase Measurements, in MEDICAL PHYSICS: Tenth Mexican Symposium on Medical Physics, Mexico City (Mexico), **1032**, 259-261 (2008)
13. Guevara E. and Gonzalez F. J., Joint optical-electrical technique for noninvasive glucose monitoring, *Revista Mexicana De Fisica*, **56(5)**, 430-434 (2010)
14. Haar T. G. and Wyard S. J., Blood cell banding in ultrasonic standing wave fields: A physical analysis, *Ultrasound in Medicine and Biology*, **4(2)**, 111-123 (1978)
15. Hill B., Accu-Chek Advantage: Electrochemistry for Diabetes Management, *Current Separations*, 45-48, <http://www.currentseparations.com> (2014)
16. <https://www.accu-chek.com/index.html> (2014)
17. International Diabetes Federation, IDF Diabetes Atlas, 6th ed., Brussels, Belgium, International Diabetes Federation (2013), <http://www.idf.org/diabetesatlas> (2014)
18. Kumar P. R., Bhansali A., Ravikiran M., Bhansali S., Dutta P., Thakur J. S., Sachdeva N., Bhadada S. K. and Walia R., Utility of glycated hemoglobin in diagnosing type 2 diabetes mellitus: a community-based study, *J Clin Endocrinol Metab*, **95(6)**, 2832–2835 (2010)
19. King L. V., On the acoustic radiation pressure on spheres, Proceedings of the Royal Society of London, **A147**, 212–240 (1934)
20. Konig K., Multiphoton microscopy in life sciences, *Journal of Microscopy*, **200(2)**, 83-104 (2000)
21. Mohan V., Shaw S. and Saboo B., Current glycemic status and diabetes related complications among type 2 diabetes patients in India: Data from the A1chieve study, *Journal of Association of Physicians of India*, **61**, 12-15 (2013)
22. Mo M., Zhong W., Zhao G., Ruan Y., Zhang H., Shi L., Lu D., Yang Q., Li Y., Jiang Q., Li R. and Xu Wang H., Combining glycosylated hemoglobin A1c and fasting plasma glucose for diagnosis of type 2 diabetes in Chinese adults, *BMC Endocrine Disorders*, **13(44)**, 1-8 (2013)
23. Mendelson Y., Pulse oximetry: theory and applications for noninvasive monitoring, *Clin. Chem.*, **38**, 1601–1607 (1992)
24. Nathan D. M. et al, *New Eng. J. Med.*, **310**, 341 - 346 (1984)
25. Perry R. C., Shankar R. R., Fineberg N., McGill J. and Baron A. D., HbA1c measurement improves the detection of type 2 diabetes in high-risk individuals with non diagnostic levels of fasting plasma glucose: the Early Diabetes Intervention Program (EDIP), *Diabetes Care*, **24(3)**, 465–471 (2001)
26. Petersson F., Nilsson A., Holm C., Jonsson H. and Laurella T., Separation of lipids from blood utilizing ultrasonic standing waves in microfluidic channels, *The Analyst, The Royal Society of Chemistry*, **129**, 938-943 (2004)
27. Radel S., Brandstetter M. and Lendl B., Observation of particles manipulated by ultrasound in close proximity to a cone-shaped infrared spectroscopy probe, *Ultrasonics*, **50**, 240–246 (2010)
28. Srivastava A., Chowdhury Md. K., Sharma S. and Sharma N., Blood Glucose Monitoring Using Non Invasive Optical Method: Design Limitations and Challenges, *International Journal of Advanced Research in Electrical, Electronics and Instrumentation Engineering (IJAREEIE)*, **2(1)**, 615-620 (2013)
29. Syed I. A., Glycated haemoglobin; past, present, and future are we ready for the change, *J Pak Med Assoc*, **61(4)**, 383–388 (2011)
30. Srivastava A., Chowdhury Md. K., Sharma S. and Sharma N., Optical Clearance Effect Determination of Glucose by near Infrared Technique: An Experimental Study using An Intralipid Based Tissue Phantom, *International Journal of Advances in Engineering & Technology (IJAET)*, **6(3)**, 1097-1108 (2013)
31. Srivastava A., Chowdhury Md. K., Sharma S. and Sharma N., Measurement of Glucose Concentration using Amplitude Modulated Ultrasound with Infrared Technique in Intralipid Phantoms and Human Whole Blood mixed intralipid phantom of Healthy and Diabetic Subjects, *Bioscience Biotechnology Research Asia*, **11(2)**, 593-602 (2014)
32. Special issue on non-invasive glucose monitoring with optical technique, *IEEE Leos Newsletter*, April (1998)
33. Tenhunen J., Kopola H. and Myllyla R., Non-invasive glucose measurement based on selective near infrared absorption: requirements on instrumentation and special range, *Measurement*, **24**, 173–177 (1998)
34. Trivelli L. A., Ranney H. M. and Lai H. T., *New Eng. J. Med.* **284**, 353 (1971)
35. Yosioka K. and Kawasima Y., Acoustic radiation pressure on a compressible sphere, *Acoustica*, **5**, 167–173 (1955).

(Received 18th August 2014, accepted 05th October 2014)

पेटेंट कार्यालय
का
शासकीय जर्नल

**OFFICIAL JOURNAL
OF
THE PATENT OFFICE**

निर्गमन सं. 03/2013
ISSUE NO. 03/2013

शुक्रवार
FRIDAY

दिनांक: 18/01/2013
DATE: 18/01/2013

पेटेंट कार्यालय का एक प्रकाशन
PUBLICATION OF THE PATENT OFFICE

(12) PATENT APPLICATION PUBLICATION

(21) Application No.3877/DEL/2012 A

(19) INDIA

(22) Date of filing of Application :14/12/2012

(43) Publication Date : 18/01/2013

(54) Title of the invention : NON INVASIVE BLOOD GLUCOSE METER BASED ON MOUDULATED ULTRASOUND & OPTICAL TECHNIQUE.

(51) International classification	:G03B 42/06	(71) Name of Applicant : 1)DR. NEERAJ SHARMA Address of Applicant :SCHOOL OF BIOMEDICAL ENGINEERING IIT (BHU), VARANASI, UTTAR PRADESH. PIN-221005. India
(31) Priority Document No	:NA	
(32) Priority Date	:NA	
(33) Name of priority country	:NA	
(86) International Application No	:NA	(72) Name of Inventor :
Filing Date	:NA	1)DR. NEERAJ SHARMA
(87) International Publication No	: NA	2)DR.SHIRU SHARMA
(61) Patent of Addition to Application Number	:NA	3)MD KOUSHIK CHOWDHURY
Filing Date	:NA	4)ANUJ SRIVASTAVA
(62) Divisional to Application Number	:NA	
Filing Date	:NA	

(57) Abstract :

A truly new technique for non invasive glucose measurement is the need of hour. Precise in vivo blood glucose level monitoring skill would be precious for robust management of diabetes in all age group of patients. None of the existing principles offer enough accuracy to replace finger prick technology. Our method utilizes modulated ultrasound & optical technique (light of wavelength in the range of visible to infrared band). Amplitude modulated ultrasonic waves are used to excite the finger, as a result different constituent molecules vibrates at their specific response frequency depending upon their weight, shape & size, these specific vibrations are detected using light, the output response signal is in the form of modulated light signal, that carries information about the concentration of different constituent molecules. This modulated light response signal is collected using photo-sensor, and suitably processed using signal processing algorithm to extract the information of blood glucose level.

No. of Pages : 13 No. of Claims : 7